

Design and Development of a Robotic System for Hand's Wrist-Fingers Rehabilitation

Fatemeh Mohandesi¹, Alireza Mirbagheri^{2,3,*}, Hamid Khabiri², Mohamad M. Mirbagheri^{2,4},
Noureddin N. Ansari^{5,6}, Maryam Norouzi⁷, Rouzbeh Kazemi, M.D⁸, Mehrnaz Aghanouri²

1: Department of Computer and Biomedical Engineering, Ahar Branch, Islamic Azad University, Ahar, Iran.

2: Department of Medical Physics and Biomedical Engineering, Medical School, Tehran University of Medical Science, Tehran, Iran.

3: Research Centre for Biomedical Technologies and Robotics (RCBTR), Advanced Medical Technologies and Equipment Institute (AMTEI), Tehran University of Medical Sciences, Tehran, Iran.

4: Department of Physical Medicine and Rehabilitation, Northwestern University, USA.

5: Research Center for War-Affected People, Tehran University of Medical Science, Tehran, Iran.

6: Department of Physiotherapy, School of Rehabilitation, Tehran University of Medical Science, Tehran, Iran.

7: Research Assistant, Electrical Engineering Department, University of Rhode Island, USA.

8: Technical Director of Tabassom Stroke Rehabilitation center.

* Corresponding author: Alireza Mirbagheri is with the Department of Medical Physics and Biomedical Engineering, School of Medicine and joint affiliated with Research Center for Biomedical Technologies and Robotics (RCBTR), Advanced Medical Technologies and Equipment Institute (AMTEI), Tehran University of Medical Sciences (TUMS), Number 21, Daneshgah St. Vali-E-Asr Ave., Tehran, Iran. (Phone: 0098-21-64053245; Mobile:; fax: 0098-21-66482654; e-mail: a-mirbagheri@tums.ac.ir).

Abstract

Hand impairment, followed by stroke, causes significant deficits in performing different activities. Restoration of hand functions requires regular and repetitive therapy exercises. Although robotically physiotherapy systems have shown great promise in hand functions' improvements, they are not widely and effectively used, as the needs and expectations of patients and physiotherapists have been ignored. In this paper, a 4-Degrees of freedom desktop-mounted robot is developed for four fingers and wrist rehabilitation, based on clinical observations. HandRoboHab provides the four mechanotherapy prevalent movements as follows: active, passive, active-assisted, and active resisted. In this study, the design and development of the robot are described. Then the efficiency and usability of the device are evaluated through two technical tests, and a preliminary clinical trial. The results of technical tests showed that HandRoboHab was able to cover the wrist range of motion of 99 to 203 degrees. Besides, the proposed device was capable of compensating its weight, which is a necessary step to accomplish the active modes exercises. In addition, clinical trial results showed that HandRoboHab was both operative and comfortable for patients with different hand sizes.

Keywords: robotically physiotherapy, stroke, hand, clinical trials, technical tests

1- Introduction

Different neurological consequences such as motor sensory, cognitive, language, and emotional disorders are followed by stroke, which is the second cause of death worldwide. Although the mortality rate due to stroke has been decreased, it is still the main cause of long-term disability. Post-stroke survivors suffer from exacerbation of hand functions as the human hand is one of the most complex limbs in terms of functionality and degrees of freedom [1–3].

The Stroke Alliance for European has declared that every 20 seconds a new stroke case occurs in adults. It has been predicted that the number of affected people by stroke will increase by 35% to 12 million in 2040 [4]. In the United States, about 800,000 subjects face stroke annually, among which 90% of the survivors are left with disability and 65% of them are not able to cooperate with their impaired hands in the different tasks even 6 months after stroke [5]. Furthermore, the exorbitant cost of rehabilitation plans and transportation, along with the lack of dexterity and strength of therapists have made the conventional methods difficult. The other drawback of

conventional methods is time-consuming along with tediousness for both patients and therapists. Finally, quantitative and accurate data of the hands' performance improvements cannot be obtained [6].

Throughout the previous decade, Robot-Assisted Training (RAT), has been utilized to improve motor deficiencies in post-stroke survivors. In this regard, different models have been created. One of the most common groups of these devices is Exoskeletons, such as M3ROB which is a robotic platform for wrist and hand [7], a lightweight exoskeleton based on hand kinematic model [1], an exoskeleton for wrist-finger [8], a three-degrees of freedom exoskeleton [9], an exoskeleton for the thumb, index, middle and ring fingers [10], FlexoHand [11], a passive exoskeleton for wrist and forearm [12], a wrist exoskeleton [13], HandMate [14], a cable-driven exoskeleton [15], and a hand exoskeleton with series elastic actuation [16]. A wide range of these devices has been created just for fingers such as a finger exoskeleton [17], a linkage finger exoskeleton [18], a magnetic-force-based for paralyzed fingers [19], a portable hand rehabilitation finger [20] and a finger extensor [21]. Another group in this field refers to soft robotic devices which are often glove-shaped, such as SEG (Soft Exoskeleton Glove) [22], hand re-extensor with steel ribbons [5], mirroring glove [23], a soft rehabilitation robot which holds continuous passive motion mode [24] and a wearable exoskeleton glove [25]. The last introduced category refers to desktop-mounted models such as parallel robotic system [26], an end-effector bilateral rehabilitation system [27], end-effector type desktop robot [28], wrist-forearm desktop robot [29], and CUBE, a cable-driven parallel structured robot desktop [30].

Although there are a great number and variety of hand physiotherapy robots, only a few of them have been widely and effectively used. In other words, robot-assisted physiotherapy, which has shown great promise in hand-function improvements, has not yet replaced conventional physiotherapy. This problem has some reasons: first, the complexity of the robot configuration makes it unusable. Second, the needs of physiotherapists and patients have been ignored. This negligence would lead to creating a device with less effectiveness on the patients, and also not being very practical for the physiotherapists.

To meet these challenges, a desktop-mounted physiotherapy system, "HandRoboHab", is proposed in this paper. This device is introduced with a simple mechanical structure and can be

used for the wrist and four fingers. To satisfy both physiotherapists' and patients' needs, the design is based on clinical observations. The main novel features of the robot are summarized as:

- 1- This device is usable for both right and left hands.
- 2- The 4 degrees of freedom are created by using just one actuator.
- 3- This device is provided with four mechano-therapy movements which are the fundamental treatments in physiotherapy.
- 4- The proposed device can be used for the deformed hand, either. Therefore, it will be utilizable for a vast range of patients. To prove the robot's features, technical and clinical tests are conducted.

The rest of the paper is comprised of six sections. In section 2, the methodology including the mechanical structures and electrical components, is explained. The control strategy for four mechano-therapy modes is described in section 3. In section 4, the results of technical and clinical tests are described. The discussion and conclusion are stated in sections 5 and 6, respectively.

2. Methodology

2.1. Clinical Observations and design requirements

In the first phase, physiotherapy observations and movement analyses were done to identify impairments of the affected hand. Afterward, the appropriate movement therapy was selected to target these impairments. The results showed that hand spasticity was the main problem of stroke survivors. Spasticity keeps the wrists and fingers in flexion position; therefore, the therapist has to re-extend them regularly during each exercise which may interrupt the current task. This intermittent job is shown in Figure 1.

Due to the spasticity differences among the individual's fingers, hand re-opening is a tedious task for physiotherapists. To address this impairment using the proposed robotic system, exerting flexion-extension movements on the four fingers and wrist were chosen. Furthermore, stretching the flexor muscles in the forearm has a great impact on spasticity reduction. Thus, this movement is also considered as one of the aims of the proposed device. These selected movements will be

achieved in all fundamental physiotherapy modes: passive, active-assisted, active and active-resisted.

2.2. Mechanical and electrical structure

The functional requirements, resulted from the previous phase, lead to the construction of the device with 1-active and 3-passive degrees of freedom to exert selected movements on the fingers-wrist. In this regard, the proposed device is composed of three main parts: 1-an adjustable finger cover and its side shafts, 2-a linear guide and 3-the driving unit.

1- Finger cover

The finger cover consists of two separated up-down segments called digit supporters, in which two phalanxes of the four fingers can be placed. The digit supporters are adjustable in length and thickness to fulfill the biomechanical compatibility with different fingers' sizes. On the other hand, the digit supporters can be used for both left and right hands. This will be achieved by rotating the finger cover structure 180 degrees. Two shafts are screwed at both sides of the finger cover. The hand cover, digit supporters, and the side shafts are shown in Figure 2.

The shafts are inserted in articulated bearings, which are connected to the linear guide wagon set via a connecting piece. The articulate bearing allows rotation of the shafts around the endpoint of the shaft, which is perpendicular to the palm.

2- Linear Guide

Two linear guides and wagons are connected to the digit supporter's side shafts, which can provide both linear and rotational movements of the fingers.

This mechanism would create three passive degrees of freedom: a translational movement of finger cover along the linear guide, the rotation of shafts around their longitudinal axis, and a rotation around the vertical axis.

3- Driving unit

The driving unit is comprised of a DC motor(Maxon, 118755,Switzerland) a position controller (Maxon, Encoder MR type ML), a power supply(QUINT-PS/10-2866763), and an amplifier (Dynamic strain Amplifier, DN-AM100 DACELL, South Korea).

The DC motor provides an active degree of freedom which is a rotation of the mechanical arm around the sagittal axis. The overall degrees of freedom created by the device and the displacement of fingers and forearms are depicted in Figure 3.

Furthermore, the robot is equipped with a force sensor, (Loadcell Zemic 1-S-B, Netherlands) to control the robot. To counteract the spasticity differences in the fingers, a constant force spring is used on both linear guides, which pulls the finger cover to fit the palm size.

To keep the patient in an ergonomic position, a specific design is made on the forearm part of the device, in which the forearm can be placed at an angle of 30 degrees to the horizon. This angle is determined based on clinical observations. For safety considerations, an emergency stop and an emergency button are utilized which can be used by the therapist and the patient, respectively. Based on the findings, some designs were depicted in SolidWorks 2015 (Dassult-Systems, France, 1995). Then the best prototype was selected and manufactured. The hardware platform is shown in Figure 4.

3.Control strategy

The control system was developed in such a way that the robot exerted the movements in all four mechanotherapy movements: passive, active-assisted, active and active-resisted. To make the controller user-friendly, the Graphical User Interface (GUI) was created by C# in the visual studio program, (Microsoft Cooperation, Washington, United States). In the Figure 5, the graphical user interface, for the proposed device is shown.

At the beginning of each exercise, the robot should be homed to make sure it would start moving from a pre-defined position, Figure 6-a shows the home position of the robot arm. Since, in the active modes the patient would displace the robot arm by his strength, the weight of the robot arm must be compensated and not imposed on the patient's hand. On the other hand, the angle of the robot arm would change while moving, which is illustrated in Figure 6-b, therefore the portion of robot arm weight which would be sustained by the hand, changes constantly. A calibration stage was done to determine the weight of the robot arm at any angle. The aim of this

calibration is to find the relation between the force corresponding to the robot's weight torque and its position (the robot angle).

The calibration stage and control algorithm for each mode is explained in the following subsections. Figure 7 shows the procedure for utilizing the device.

3.1. Calibration

For the calibration, the robot moved in a quasi-static mode, at a very slow speed without carrying the user's hand. In such condition, the load cell would measure the torque resulting from the pure weight of the robot in any direction. The robot angles were also recorded using the encoder. By dividing the measured torque by the torque arm, the obtained force corresponding to each robot position is plotted in Figure 8. To extract the relation, the curve fitting tool of MATLAB was used and the equation 1 was obtained.

$$F_{wt} = 22.64 \sin((0.020 \times Angle) + 1.701) \quad (1)$$

3.2. Passive mode

In this mode, the motor moves the robot arm with a constant velocity specified by the user, until the current position is the same as the final position. Figure 9 illustrates all the control algorithms. After that, the direction of the motor rotation is reversed and the robot arm comes back to its home position. To stretch the flexor muscles in the forearm, the robot arm can be stopped in the maximum position, by means of setting the stopped time. For more safety, a Max. Force option is suggested which if set, the robot would stop immediately when it reaches the force set value. The robot's range of motion can be adjusted by the min. pos. and max. pos. options on the GUI.

3.3. Active mode

To perform the active mode, the device calibration data is used to compensate the robot's weight. The motor moves with a velocity commensurate with the weight obtained from the calibration based on the current angle. As the user changes the robot's position by applying a

force, its weight changes. The new weight is read using the calibration formula and the new motor velocity is calculated.

3.4. Active-Assisted mode

In this mode, the difference between the force shown by the load cell (F_L), and the robot's weight corresponding to the current position is calculated, (F_u). F_L is the summation of the robot weight (F_W) and the user's force. According to this difference, the motor moves with a velocity proportional to F_W , or it moves with a velocity proportional to F_u .

3.5. Active-Resisted mode

To run this mode, the motor produces the torque, opposite to the hand movement direction with the help of the current control mode. The value of the motor velocity is proportional to F_u .

4. Clinical and technical tests

4.1. Technical tests

Passive mode test: A technical test is performed on the passive mode to check the capability of the device in covering a standard wrist range of motion. To this end, a healthy subject trained with the robot in passive mode and the wrist range of motion is calculated. The angle of the robot changes from 0 to 110 degrees, set in the GUI, with an increment of 5°. At each angle, the real angle of the wrist is measured. Table 1 shows the results of the passive mode test.

Active mode test: Another technical test is performed to check the capability of the robot in compensating its weight while performing in the active mode. To perform this test, another load cell (1-B-S-50Kg.0.2B, Zemic, Netherlands) is attached to the connector piece. This new setup is shown in Figure 10.

By applying a finger force on this loadcell and moving the robot arm, periodically, two series of data are collected: the force monitored by the external loadcell and the torque measured by the internal loadcell. The force which is sensed by the internal sensor would be calculated by dividing the internal load cell output by the torque arm. Figure 11 shows these two forces.

4.2. Clinical tests

To find any possible problem that may occur during the rehabilitation, the device is tested on five healthy subjects. None of them were reported to encounter a serious problem while exercising with the device. Afterward, the test is conducted on 10 post-stroke patients, within the age range of 21-70, and with left-side affected. Figure 12 shows the setup and the patient exercising with the device.

The purpose of this test is to evaluate the effectiveness and usability of the device for the patients and therapists. In Table 2, the specifications of the recruited patients in this experiment have been shown. All participants were informed consent to the experiment that was approved by the Research Ethics Board of Tehran University of Medical Science (IR.TUMS.REC.1394.1505).

Testing the device on the patients shows that the most used movement mode is the passive mode. Only one patient could do the exercise in active-assisted mode. 7 of 10 patients could do the exercises well without any problem. The duration of training was adjusted with respect to the strength and ability of patients. One of the three patients, who could not practice with the device, had wrist pain in the home position due to wrist stiffness. Therefore, a higher starting position was set for him. In the other two patients, the finger cover structure and the hand were not connected well and the hand came out of the cover while moving. It was concluded from the clinical test that HandRoboHab can increase the motivation of patients in the treatment process because some of them were passionate to work with the device more than once.

5. Discussion

Neurological diseases such as CVA, can diminish the hand's performance. In this regard, various types of devices have been developed to restore hand functions [11,31,32]. In this article, we presented the design and fabrication of HandRoboHab, a therapeutic device, to exert physiotherapy movements on the wrist and fingers. The design is based on clinical observations, through which the needs of therapists and patients are extracted. Accordingly, the most important need for therapists is eliminating repetitive and tedious movements, and for the patients pivotal movements to reduce spasticity. In this regard, according to the information in [33,34], the average length and thickness of fingers are obtained and the HandRoboHab is designed, fabricated, and evaluated by conducting some technical and clinical tests.

One of the most important features of this robot is its simple structure where only one actuator is employed for 4 degrees of freedom provided by the robot, which is rarely seen among similar models. Compared to the [35] and [36] that use PAM(pneumatic artificial muscle), the components of this robot are designed to be very simple and efficient.

Besides, the robot's light weight makes it portable. The device is composed of a hand cover that can hold four fingers of different sizes and thicknesses. Another prominent feature of the proposed robot is its usability for both right and left hands, which is accomplished for the first time. Consequently, this device can be used for a wide range of patients regardless of the damaged side of the brain. Additionally, by using a force-constant spring, different spasticity among the four fingers and also among the different subjects can be compensated.

A wide range of therapeutic robots have been designed solely for finger physiotherapy [20–22] and some of them can be used just for the wrist [29,37,38]. Since simultaneous functions of the wrist and fingers along with restoring appropriate their range of motion is important for achieving hand dexterity and satisfied healing, both wrist and fingers are considered as the target for the proposed robot.

Another option that distinguishes this device from the other models is its software and control strategy. Most of the devices are CPM(Continuous Passive Motion), such as [39] ,[40] , and can exert only passive motions. In the presented prototype, four mechano-therapy movements would be created. Consequently, the HandRoboHab can be used not only for post-stroke patients but also for any neurological deficit.

To investigate the device's ability to cover an acceptable wrist range of motion, the passive mode test, is done as explained in the section. It can be seen from Table 3 that the device can rehabilitate the wrist in the range of 99 to 203 degrees. In the active mode test, the robot weight compensation ability is approved. By comparing the two graphs shown in Figure 11, it can be observed that the force corresponding to the internal load cell output follows the force calibration diagram. The finger forces shown in Figure 11-a add the disturbance-shaped signals to the force resulting from the weight signal, Figure 11-b. Since the main load cell measures both the user force and robot weight at each angle, it can be inferred that the weight is not borne by the user and is compensated by the motor.

For the clinical test, the device is tested on both healthy and post-stroke patients. The results show the usability and effectiveness of the device for both patients and therapists.

6.Conclusion

In this paper, a desktop robotic system is introduced with 4-DOFs, which are actuated by only one actuator, with the aim of rehabilitation of the wrist and four fingers. The system design satisfies the requirements of all physiotherapy movements: passive, active-assisted, active, and active resisted. This device is designed and fabricated based on patients' and therapists' needs. Besides, some important items such as velocity, time, and force are precisely controlled. All of these specifications bring great potential for its further clinical applications.

The tests on healthy subjects and patients show that this device can be a good alternative to conventional therapies and is widely used in rehabilitation centers, due to the satisfaction of patients and physiotherapists. The patients show great motivation in utilizing this device and physiotherapists are satisfied when working with the device.

To show the effects of the robot on the disease process and the rate of improvement in patients, more extensive clinical tests will be performed and the results of exercises with this robot can be seen in stroke patients.

Acknowledgment-

This project, design and fabrication, was supported by the Tehran University of Medical Science (grant number 30212-30-0394). The authors would like to acknowledge the Research Center for Biomedical Technologies and Robotics (RCBTR), for the generous support for this research.

References

1. Guo, K., Lu, J., Liu, C., et al., “Development, Research, Optimization and Experiment of Exoskeleton Robot for Hand Rehabilitation Training”, *Appl. Sci.*, **12**(20), p. 10580 (2022).
2. Sung, Y., Lee, D. and Lee, J., “Descriptive Study on Rehabilitation Treatment and Evaluation Methods for Improving Upper Limb Function in Stroke Patients”, **12**(19), p. 39 (2020).
3. Bharati, B., Sahu, S., and Pati, S., “Rehabilitation of Stroke Patients in India: An Exploratory Study from a National-Level Survey Data”, *Indian J. Physiother. Occup. Ther.*, **15**(3) (2021).
4. Hernandez, M., Lopez, B., Sanchez, A., et al., “Effects of Specific Virtual Reality-Based Therapy for the Rehabilitation of the Upper Limb Motor Function Post-Ictus: Randomized Controlled Trial. *Brain Sci.* 2021, 11, 555” (2021).
5. Rieger, C. and Desai, J., “A Preliminary Study to Design and Evaluate Pneumatically Controlled Soft Robotic Actuators for a Repetitive Hand Rehabilitation Task”, *Biomimetics*, **7**(4), p. 139 (2022).
6. Bouteraa, Y., Ben-Abdallah, I., and Boukthir, K., “A New Wrist-Forearm Rehabilitation Protocol Integrating Human Biomechanics and SVM-Based Machine Learning for Muscle Fatigue Estimation”, *Bioengineering*, **10**(2), p. 219 (2023).
7. Cisnal, A., Cagigal, V., Liraje, G., et al., “An Overview of M3Rob, a Robotic Platform for Neuromotor and Cognitive Rehabilitation Using Augmented Reality” (n.d.).
8. Mandeljc, A., Rajhard, A., Munih, M., et al., “Robotic Device for Out-of-Clinic Post-Stroke Hand Rehabilitation”, *Appl. Sci.*, **12**(3), p. 1092 (2022).
9. Shalal, S. and Aboud, S., “Smart Robotic Exoskeleton: a 3-DOF for Wrist-forearm Rehabilitation”, *J. Robot. Control*, **2**(6), pp. 476–483 (2021).

10. Bauer, O., Vizi, B., Galambos, P., and Szalay, T., “Direct Drive Hand Exoskeleton for Robot-assisted Post Stroke Rehabilitation”, *Acta Polytech. Hungarica*, **18**(5), pp. 37–54 (2021).
11. Ahmed, T., Zaman, U., Islam R., et al., “Flexohand: A Hybrid Exoskeleton-Based Novel Hand Rehabilitation Device”, *Micromachines*, **12**(11), p. 1274 (2021).
12. Kutuk, E., Dulger, C. and Das, T., “Design of a robot-assisted exoskeleton for passive wrist and forearm rehabilitation”, **10**(1), pp. 107–118 (2019).
13. Lin, H., Su, Y., Lai, H., et al., “A Spatial-Motion Assist-as-Needed Controller for the Passive, Active, and Resistive Robot-Aided Rehabilitation of the Wrist”, **8**, pp. 133951–133960 (2020).
14. Sandison, M., Phan, K., Casas, R., et al., “HandMATE: Wearable Robotic Hand Exoskeleton and Integrated Android App for At Home Stroke Rehabilitation”, *2020 42nd Annu. Int. Conf. IEEE Eng. Med. Biol. Soc.*, IEEE, pp. 4867–4872 (2020).
15. Amin, H., Assal, M., and Iwata, H., “A new hand rehabilitation system based on the cable-driven mechanism and dielectric elastomer actuator”, **11**(2), pp. 357–369 (2020).
16. Marconi, D., Baldoni, A., McKiney, Z., et al., “A novel hand exoskeleton with series elastic actuation for modulated torque transfer”, *Mechatronics*, **61**, pp. 69–82 (2019).
17. Norouzi, M., Karimpour, M., and Mahjoob, M., “A Finger Rehabilitation Exoskeleton: Design, Control, and Performance Evaluation”, *2021 9th RSI Int. Conf. Robot. Mechatronics*, IEEE, pp. 301–308 (2021).
18. Bohme, M., Kohler, P., Thiel R., et al., “Preliminary Biomechanical Evaluation of a Novel Exoskeleton Robotic System to Assist Stair Climbing”, *Appl. Sci.*, **12**(17), p. 8835 (2022).
19. kim, H., Ji, M., Kim, Y., et al., “Therapeutic Effects of a Newly Developed 3D Magnetic Finger Rehabilitation Device in Subacute Stroke Patients: A Pilot Study”, *Brain Sci.*, **12**(1), p. 113 (2022).
20. Zhu, X. and He, B., “Underactuated Rehabilitation Robotics for Hand Function”, *J. Robot. Control*, **2**(5), pp. 337–341 (2021).
21. Shahdad, I., Azlan, Z., and Jazlan, A., “Modelling a 1-DOF Finger Extensor Machine for

Hand Rehabilitation”, *IIUM Eng. J.*, **22**(2), pp. 384–396 (2021).

22. Kladovasilakis, N., Kostavelis, I., Sideridis, P., et al., “A Novel Soft Robotic Exoskeleton System for Hand Rehabilitation and Assistance Purposes”, *Appl. Sci.*, **13**(1), p. 553 (2022).

23. Kim J., Lee G., Jo H., et al., “A Wearable Soft Robot for Stroke Patients’ Finger Occupational Therapy and Quantitative Measures on the Joint Paralysis”, pp. 1–8 (2020).

24. Ying, Z., Al-Shammari, K., Faudzi, A., et al., “Continuous Progressive Actuator Robot for Hand Rehabilitation”, **10**(1), pp. 5276–5280 (2020).

25. Gerez, L., Gao, G., Dwivedi, A., et al., “A Hybrid, Wearable Exoskeleton Glove Equipped With Variable Stiffness Joints, Abduction Capabilities, and a Telescopic Thumb”, **8**, pp. 173345–173358 (2020).

26. Tohanmean, N., Tucan, P., Vanta, M., et al., “The Efficacy of the NeuroAssist Robotic System for Motor Rehabilitation of the Upper Limb—Promising Results from a Pilot Study”, *J. Clin. Med.*, **12**(2), p. 425 (2023).

27. Jiao, R., Liu, W., Rashad, R., et al., “A Novel Robotic System Enabling Multiple Bilateral Upper Limb Rehabilitation Training via an Admittance Controller and Force Field” (2023).

28. RahmanKhan, M., Ahmed, T., Pallares, J., et al., “Development of A Desktop-mounted Rehabilitation Robot For Upper Extremities” In *4th International Conference on Industrial & Mechanical Engineering and Operations Management*.

29. Kuryto, P., Cyganiuk, J., Frankovsky, P., et al., “Wrist Rehabilittation with Manipulator to Perform Passive and Active Exercises”, **49**(2), pp. 52–57 (2019).

30. Cafolla, D., Russo, M., and Carbone, G., “CUBE, a Cable-driven Device for Limb Rehabilitation”, *J. Bionic Eng.*, **16**(3), pp. 492–502 (2019).

31. ALmusawi, H. A., “Design and Development of a New Hand and Wrist Rehabilitation Robot-Assisted System; Equipped With Game-Based Therapy, ROM and Tip-Pinch Force Self-Assessment Approaches”.

32. Baldan, F., Turolla, A., Rimini, D., et al., “Robot-assisted rehabilitation of hand function

after stroke: Development of prediction models for reference to therapy”, *J. Electromyogr. Kinesiol.*, **57**, p. 102534 (2021).

33. Kim, H. and Kim, G.-S., “Development of a finger-rehabilitation robot for fingers’ flexibility rehabilitation exercise”, *Int. J. Precis. Eng. Manuf.*, **14**(4), pp. 535–541 (2013).
34. Tang, Z., Sugano, S., and Iwata, H., “A novel, MRI compatible hand exoskeleton for finger rehabilitation”, *Syst. Integr. (SII), 2011 IEEE/SICE Int. Symp.*, IEEE, pp. 118–123 (2011).
35. Tjahyono, P., Aw, C., Devaraj, H., et al., “A five-fingered hand exoskeleton driven by pneumatic artificial muscles with novel polypyrrole sensors”, *Ind. Robot An Int. J.*, **40**(3), pp. 251–260 (2013).
36. Xing K., Xu Q., He J., et al., “A wearable device for repetitive hand therapy”, *Biomed. Robot. Biomechatronics, 2008. BioRob 2008. 2nd IEEE RAS EMBS Int. Conf.*, IEEE, pp. 919–923 (2008).
37. Lambelet, C., Lyu, M., Wooley, D., et al., “The eWrist—A wearable wrist exoskeleton with sEMG-based force control for stroke rehabilitation”, *Rehabil. Robot. (ICORR), 2017 Int. Conf.*, IEEE, pp. 726–733 (2017).
38. O'Malley, K., Burgar, C., Sledd, A., et al., “The RiceWrist: A distal upper extremity rehabilitation robot for stroke therapy”, *ASME 2006 Int. Mech. Eng. Congr. Expo.*, American Society of Mechanical Engineers, pp. 1437–1446 (2006).
39. HealthCare, “Waveflex hand CPM device”. Available: <https://www.remingtonmedical.com/product/waveflex-cpm/> (2019)
40. “KINETECTM MaestraTM Hand & Wrist CPM Machine”. Available: <https://www.scribd.com/document/317675512/Catalog-Kinetec-pdf/> (2019)

Figure 1. Spasticity compensation and forearm traction exercises

Figure 2. (a).The CAD model of digit supporters and the side shafts. (b). real model of the finger cover. (c). the real model of side shaft

Figure 3. a:(1). the finger cover. (2). the forearm placement. b: (3). active degree of freedom created by the DC motor. (4). linear movement of finger cover. (5). rotation around the vertical axis (Yaw). (6). rotation of finger cover around the latitudinal axis (Pitch).

Figure 4. The robot platform, a: 1. Encoder 2. DC motor 3. Reduction gearbox 4. coupling mechanism 5. Ball bearing, 6. loadcell 7. mechanical structures 8. power supply. 9. Position controller 10. Amplifier b: 11. Emergency stop 12. Linear Guide 13. An emergency stop button 14. Handset

Figure 5. The GUI of the device

Figure 6. (a): home position, (b):the angles of the robot at which its weights are measured

Figure 7. The procedure for utilizing the device

Figure 8. The force corresponding to the weight torque at each angle

Figure 9. The control diagram of the robot, mode1: passive, mode2: active, mode3: active-assisted, mode4: active-resisted

Figure 10. a: the whole setup for the active technical test. b: the closed view of the new sensor attachment. c- the external sensor

Figure 11. The results of the active test. (a): the output of the external load cell. (b): the force corresponding to the internal load cell output

Figure 12. a: The hardware setup for the clinical test. b: the patient's hand in the home position. c- the hand in the stretching position

Table1. The results of the passive mode technical test

Table2. The specifications of the participants (patients)



Fig.1

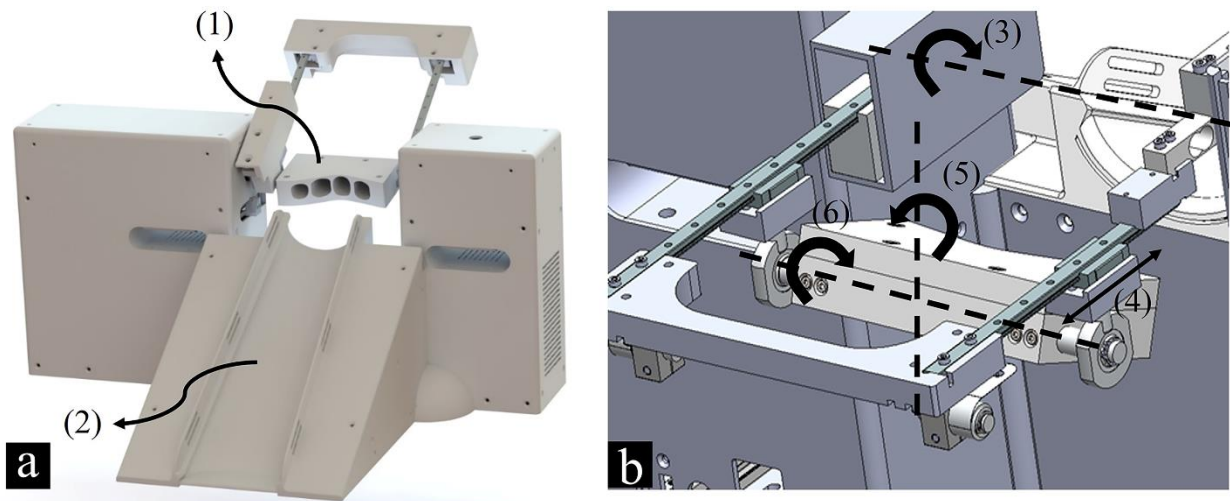


Fig.2

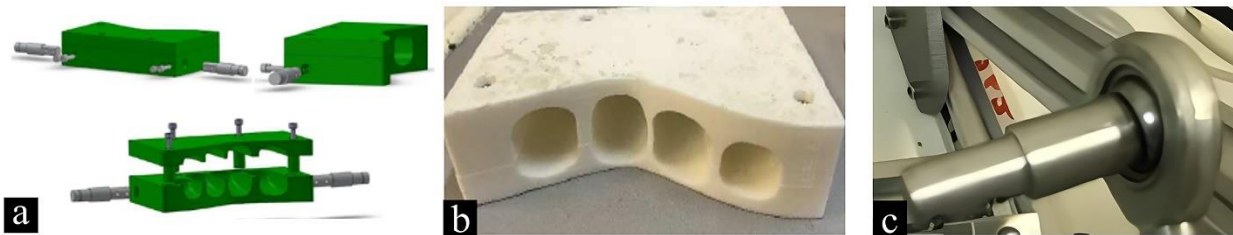


Fig.3

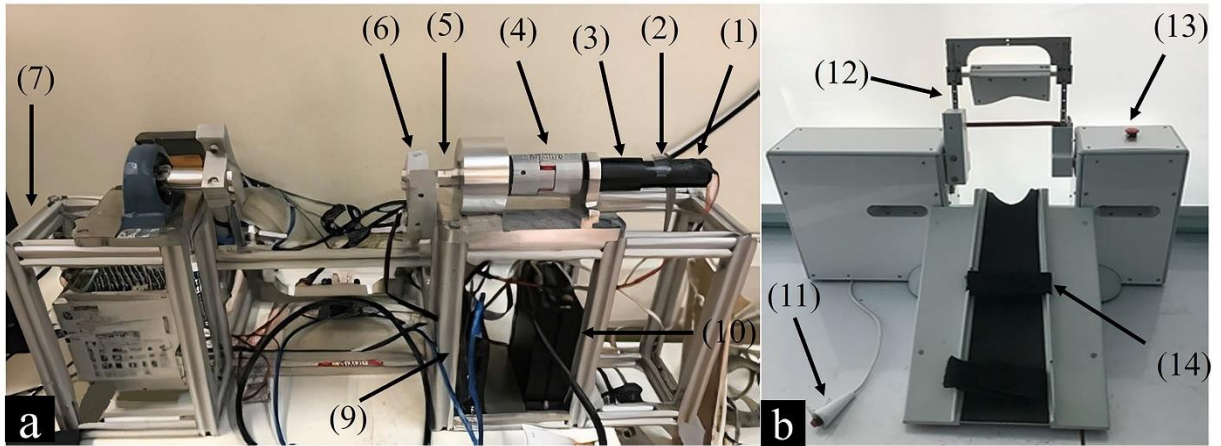


Fig.4

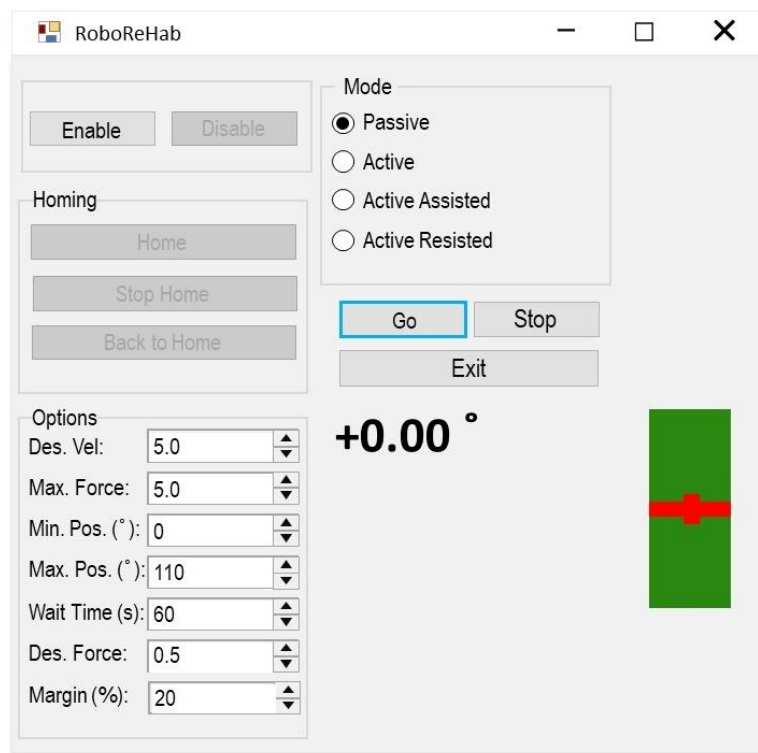


Fig.5

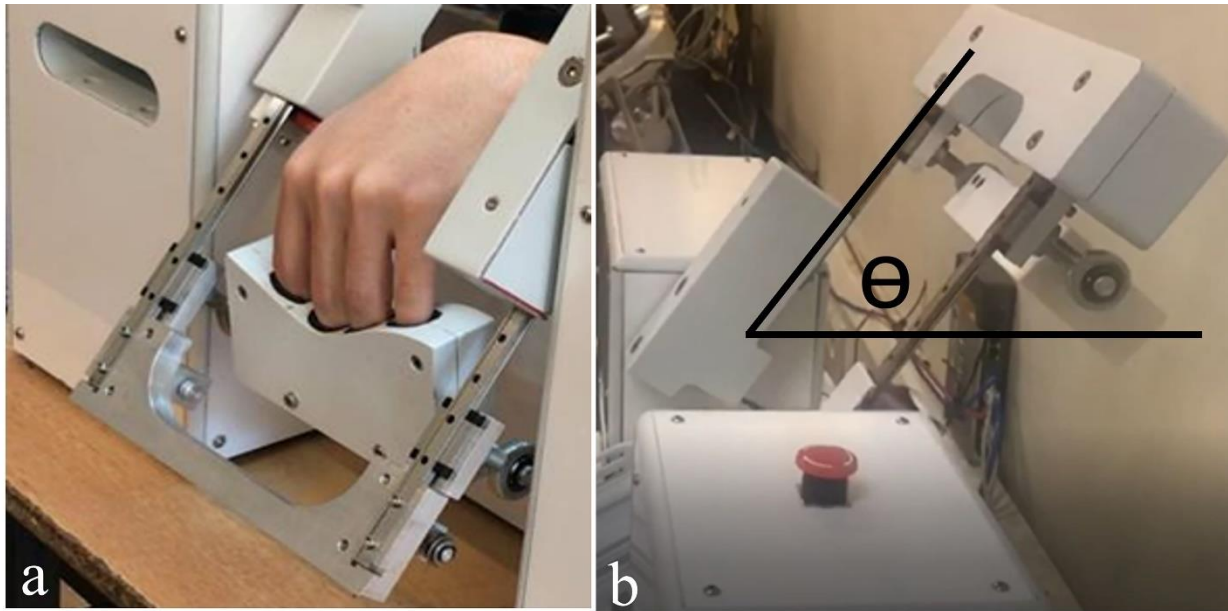


Fig.6

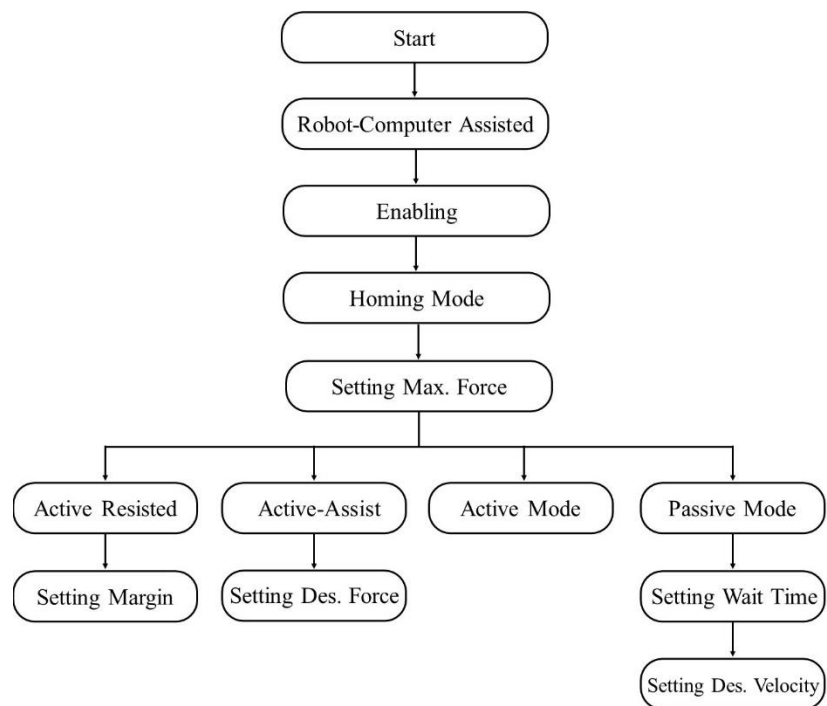


Fig.7

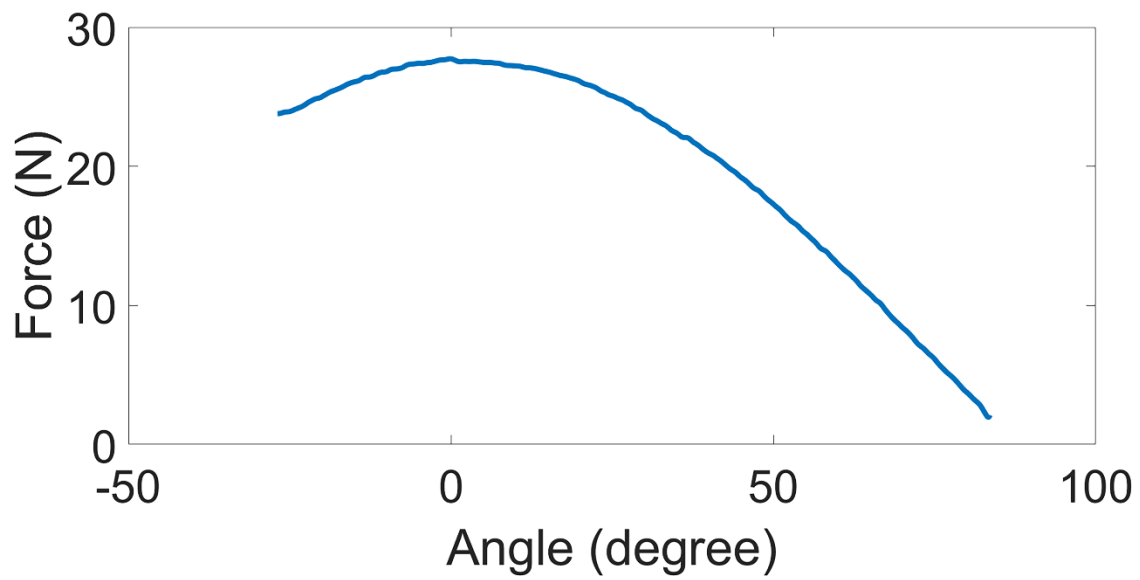


Fig.8

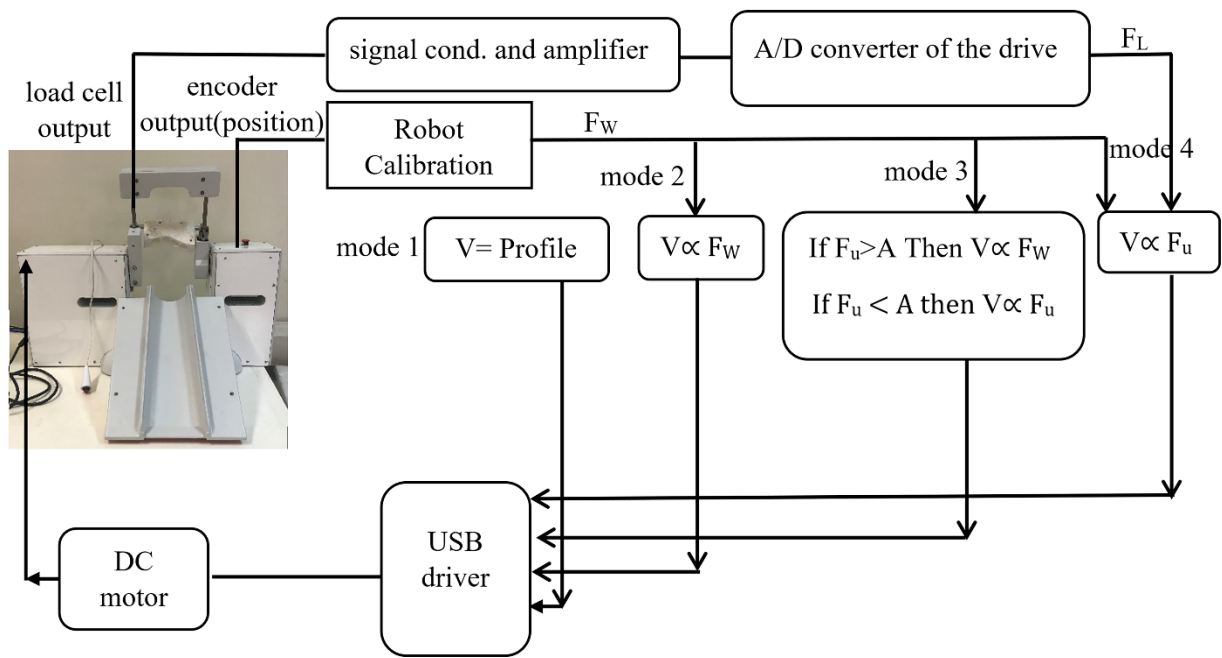


Fig.9

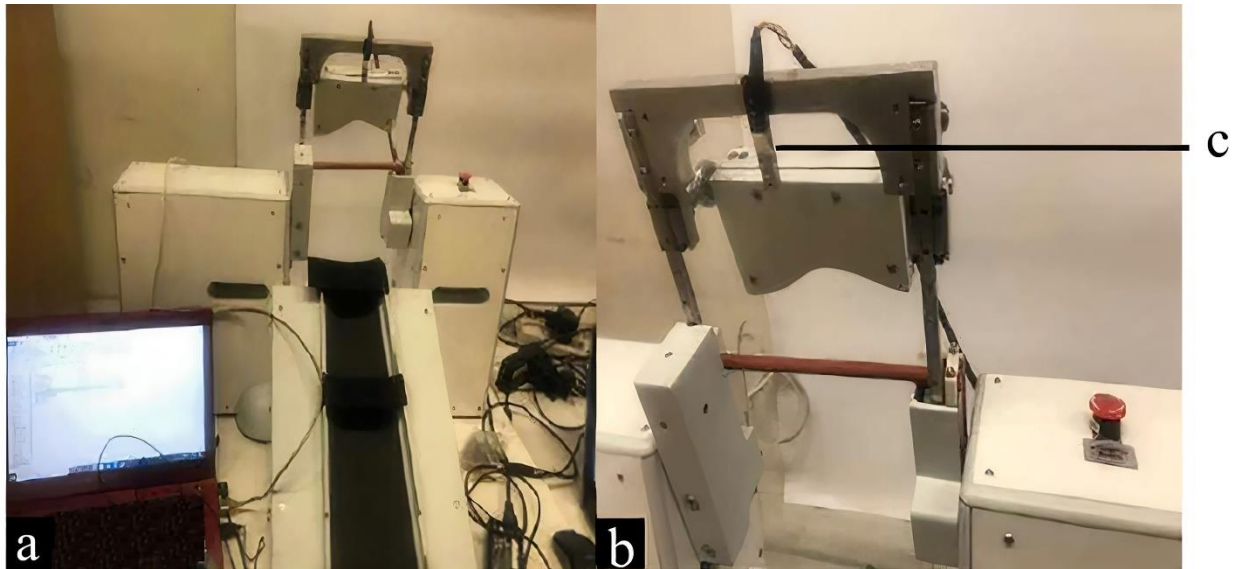


Fig.10

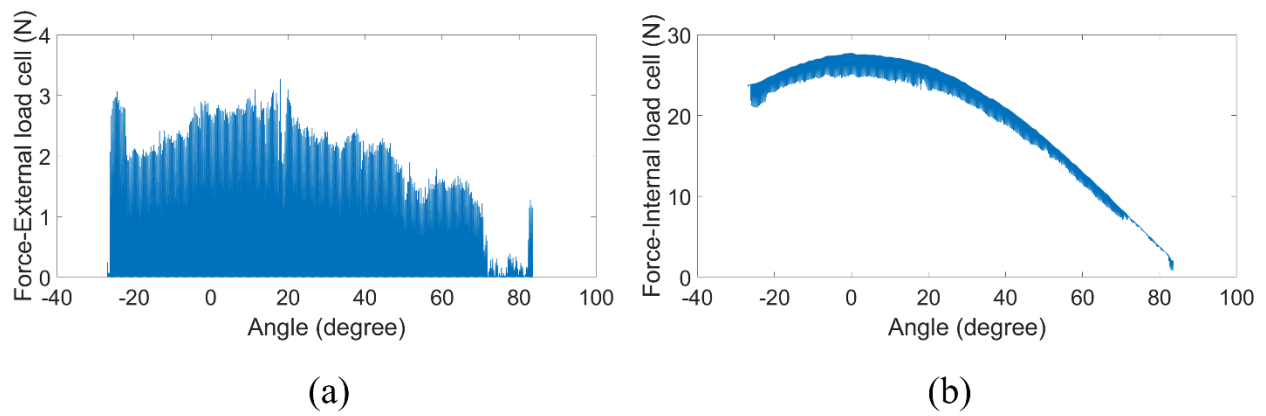


Fig.11

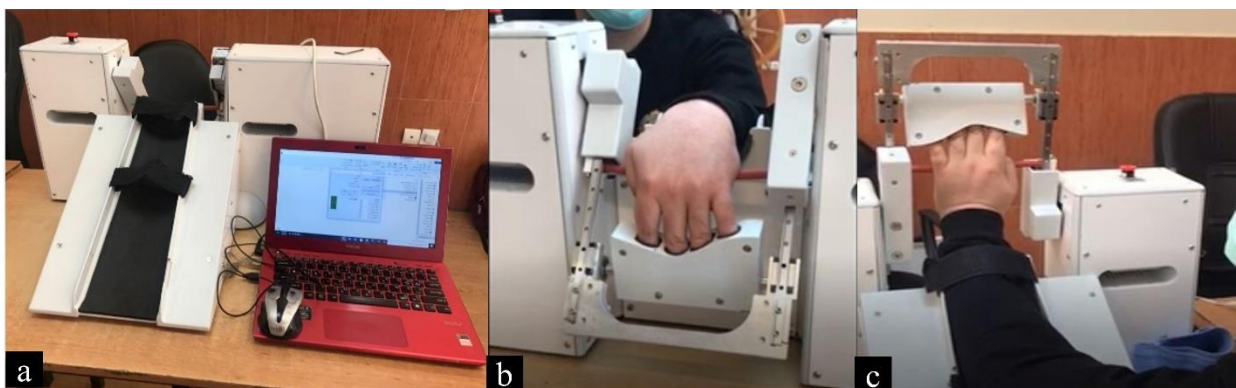


Fig.12

Table.1

Robot Angle (degrees)	Real angle measured by SolidWorks(degrees)
0- degree (home position)	99.24
0-5	106
5-10	110.01
10-15	113.14
15-20	115.23
20-25	119.51
25-30	124.97
30-35	129.33
35-40	132.39
40-45	135
45-50	140
50-55	145
55-60	149
60-65	154.57
65-70	159.93
70-75	165.80
75-80	169.20
80-85	174.13
85-90	178.90
90-95	185.90
95-100	190.67
100-105	196.20
105-110	202.80

Table.2

subjects	sex	Modes of movement therapy	Duration and number of uses	result
Subject1	female	passive	2 minutes- 1 time	Done
Subject2	female	passive	3 minutes- 1 time	Done
Subject3	female	passive	6 minutes- 2 times	Done
Subject4	male	Passive- Active assisted	5 minutes- 2 times	Done
Subject5	male	passive	5 minutes- 2 times	Done
Subject6	female	passive	5 minutes- 2 times	Done
Subject7	male	passive	5 minutes	Done
Subject8	male	passive	Less than 1 minute	Not completed, due to the wrist stiffness and pain
Subject9	male	passive	Less than 1 minute	Not completed
Subject10	female	passive	Less than 1 minute	Not completed

Biography-

Fateme Mohandesi received her bachelor of Bioelectrics (2003) and master of Biomechanics (2009) from Islamic Azad University of south branch of Tehran and Iran University of Science and Technology, respectively. She joined biomedical engineering department of Islamic Azad University, Ahar branch in 2012. She obtained her Ph.D. degree in Biomedical Engineering, Medical Robotics from Tehran University of Medical Science in 2022. She is now assistant professor of biomedical department, at Islamic Azad University, Ahar-Tabriz branch. She is interested in medical equipment, Robotics, Medical robotics, biomechanics.

Email: Fatemeh.Mohandesi@iau.ac.ir

Alireza Mirbagheri obtained his Ph.D. degree in Mechanical Engineering from Sharif University of Technology, Tehran, Iran, in 2012. Subsequently, he joined the Department of Medical Physics & Biomedical Engineering at the School of Medicine in Tehran University of Medical Sciences (TUMS) as an associate professor and deputy of research affairs. He holds a joint appointment at the Research Center for Biomedical Technologies and Robotics (RCBTR), part of the Advanced Medical Technologies and Equipment Institute (AMTEI) at TUMS. There, he serves as deputy of research affairs and director of the Robotic Surgery Lab (RSL). Dr Mirbagheri is the founder and director of Iran Advanced Clinical Training Center (IACT), as well as founder and CEO of the “Sina Robotics and Medical Innovators Co., Ltd.”, which introduced the “Sina” Robotic Tele-surgery system and the “SinaSim” simulators. Currently, his research and activities focus on designing and implementing of robotic tele-surgery systems and haptic interfaces.

Hamid Khabiri, received his Ph.D. in Biomedical Engineering from Tehran University of Medical Science (TUMS). Currently, he works as a researcher at the research center for biomedical technologies and Robotics. His interest is in designing and developing medical robotics, especially in the field of rehabilitation.

Email: khabiri.bme@gmail.com

Mehdi M. Mirbagheri holds a Ph.D. in biomedical engineering, which he earned at McGill University in Montreal, Canada. His career includes roles as a Senior Research Scientist at the Sensory Motor Performance Program at RIC and as an Associate Professor at Northwestern University. Presently, he is an Associate Professor at Tehran University of Medical Science and the founder and director of the Neural Engineering and Rehabilitation Research Center. Mirbagheri's expertise spans rehabilitation engineering, neural engineering, biomedical engineering, biological signal analysis, human movement, robotic rehabilitation, and control systems. He couples this technical prowess with extensive clinical experience and longstanding collaborations in Human Movement, with a particular emphasis on neurological disorders. Email: mehdi.northwestern@gmail.com

Nouredin Nakhostin Ansari holds a Bachelor of Science (BSc) and a Master of Science (MSc) in Physiotherapy, both obtained from the School of Rehabilitation at Tehran University of Medical Sciences (TUMS). Additionally, he earned his Doctor of Philosophy (PhD) in Physiotherapy from Tarbiat Modarres University in Iran. Currently, he serves as a distinguished

professor at the School of Rehabilitation in TUMS. His primary research interests focus on assessing muscle spasticity and neurorehabilitation, with a special emphasis on stroke rehabilitation.

Email: nakhostin@sina.tums.ac.ir

Maryam Norouzi is a Ph.D. student in the Department of Electrical, Computer, and Biomedical Engineering at the University of Rhode Island, specializing in brain-computer interfaces. Prior to her current studies, she spent three years at Sina Robotics and Medical Innovators as a Research Fellow and Mechanical Design Engineer. Maryam earned her Master's degree in Mechanical Engineering from the University of Tehran, where her primary focus was on rehabilitation exoskeletons. She received her Bachelor's degree in Mechanical Engineering from AmirKabir University.

Email: maryam_norouzi@uri.edu

Rouzbah Kazemi received his medical degree at Tehran University of Medical Sciences in 2002. He established the first physiotherapy center for neuro muscular disorders patients in 2008. He has translated 12 medical books and honored 5 patents so far.

Email: drrok9141@gmail.com

Mehrnaz Aghanouri received her bachelor of science in Mechanical engineering and master of science in Mechatronic engineering from Isfahan University of technology and K.N. Toosi University of Technology, respectively. She is currently a Ph.D. student in Medical robotics at Tehran University of Medical Sciences and a researcher at the Research Center for Biomedical Technologies and Robotics (RCBTR). Her research interests include medical robotics, human-robot interaction, image processing, machine learning, artificial intelligence, dynamics and control.

Email: m-aghanouri@razi.tums.ac.ir

Contributions-

Fatemeh Mohandesi: conceived of the presented idea, developed the theory, performed clinical observations, sketching different models by software, prototyped the device, carried out the clinical and technical test, interpreted the clinical and technical results. wrote the initial draft of article, doing the revision of the article especially the literature review and introduction.

Alireza Mirbagheri: developed the theory, sketched and evaluated different designed models, developed the control algorithm, prototyped the device and support the writing the whole manuscript.

Hamid Khabiri: performed clinical observations, prototyped the device, carried out the technical test, correct the initial draft of the manuscript, contributed in revising the article.

Mohammad Mehdi Mirbagheri: providing consultation on both clinical and technical aspects of the manuscript

Noureddin Nakhostin Ansari: conceived of the clinical and medical issues of the project, supporting additional information about post-stroke patients, provided post-stroke patients for the clinical observations, contributed in interpretations of the clinical results.

Maryam Norouzi: finalized the software model, contribute in prototyping the device and writing the manuscript.

Rouzbeh Kazemi: provided post-stroke patients in Tabasom clinic for the clinical test

Mehrnaz Aghanouri: developed the control algorithm, performed the computations, contributed in the technical test, correct the initial draft of the manuscript, contributed in revising the manuscript.