



Diagnosing and evaluating the severity of chronic obstructive pulmonary disease based on the time-frequency features of the S-transform applied to the lung sound signal

Mahsa Amin Eskandari, Saeid Rashidi *

Faculty of Medical Sciences and Technologies, Science and Research Branch, Islamic Azad University, Tehran, Iran.

* Corresponding author: rashidi.saeid@gmail.com (S. Rashidi)

Received 31 December 2022; Received in revised form 3 July 2023; Accepted 19 November 2023

Keywords

Classification;
Chronic Obstructive
Pulmonary Disease
(COPD);
Lung sound;
Stockwell transform (S-
transform);
Time-frequency features.

Abstract

Chronic Obstructive Pulmonary Disease (COPD) is a common respiratory disease characterized by chronic inflammation of the lung airways and destruction of lung tissue that leads to airflow limitation. Asthma and COPD are the two most common respiratory diseases that together cause approximately 180,000 deaths worldwide every year. Moreover, the death rate of COPD is eight times higher than the death rate of Asthma. COPD is the third leading cause of death worldwide. Time-frequency transform has been used to diagnose and evaluate the severity of this disease using recorded signals, which are dynamic and non-static. In this research, the Stockwell transform (S-transform) is used as a tool to extract features from the lung signal. S-transform has a higher frequency resolution than wavelet transforms at low frequencies, and at high frequencies, it has a lower frequency resolution but a higher time resolution. After feature extraction using the S-transform, mathematical statistics were applied to reduce feature dimensions. The results indicate that with K-fold validation for K-Nearest Neighbors (KNN) classification, the accuracy, precision, and sensitivity values are 98.39%, 97.45%, and 93.88%, respectively. For Support Vector Machine (SVM), the results are 95.23%, 92.59%, and 83.33%, respectively.

1. Introduction

Chronic Obstructive Pulmonary Disease (COPD) is a disease that is both preventable and treatable. People with this disease usually struggle to breathe more than healthy people, which causes shortness of breath. At the beginning of the disease, a person may experience symptoms such as shortness of breath during exercise. As the disease progresses, breathing, especially exhalation, becomes increasingly difficult [1]. Symptoms of COPD include shortness of breath, cough, and phlegm production. However, some patients may experience more severe symptoms such as frequent respiratory infections, chest pain, and fatigue. This disease is currently one of the leading causes of death in the world, and it is expected that the number of deaths will increase in the coming years [2].

The increasing severity of COPD indicates worsening symptoms and significant adverse outcomes for patients. Exacerbations of this disease cause increased airway and systemic inflammation and physiological changes [3].

The increase in disease severity and airway inflammation is often caused by infections. Viral infections are a major cause of this disease, although bacterial infections and environmental factors such as air pollution, geographical conditions, and ambient temperature can also contribute to COPD [4]. COPD affects more than 250 million people worldwide and has high economic costs [5]. In early childhood, severe viral and bacterial lung infections have been associated with reduced lung function and increased respiratory symptoms in adulthood,

To cite this article:

M. Amin Eskandari and S. Rashidi "Diagnosing and evaluating the severity of chronic obstructive pulmonary disease based on the time-frequency features of the S-transform applied to the lung sound signal", *Scientia Iranica* (2025) 32(19): 7440.

<https://doi.org/10.24200/sci.2023.61685.7440>

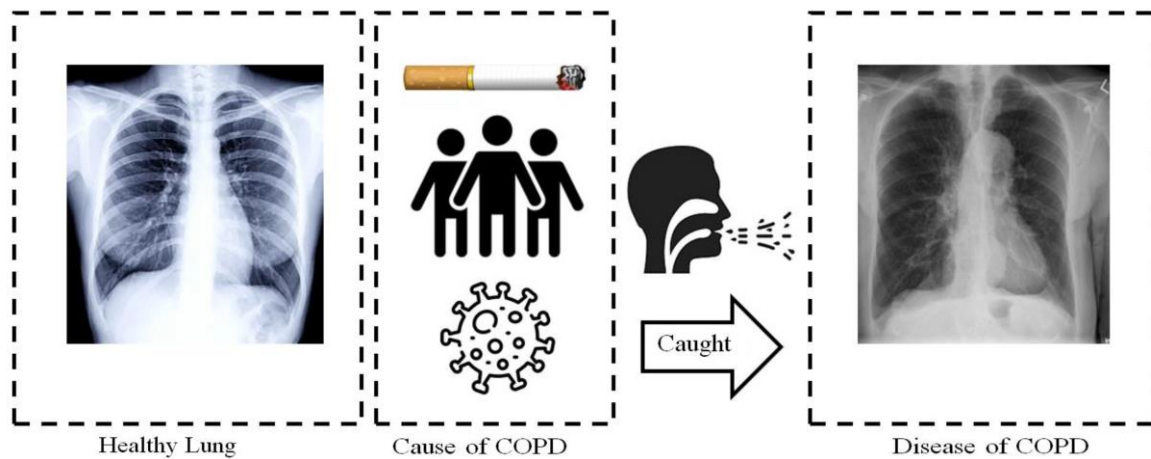


Figure 1. Overview of stages of lung involvement in people with COPD.

contributing to COPD development [6]. Sound can be produced from a person's lungs during the breathing mechanism. These sounds are classified into two categories: Normal breathing sounds and adventitious sounds. Normal breath sounds are produced with no lung problems, but wheezing and crackling sounds are usually associated with lung pathology [7]. This article presents a review of clinical auscultation as a diagnostic tool for lung diseases and the recent advances that have made it possible to obtain more objective observations compared to the past. Quantitative lung sounds are related to clinical, physiological, and radiological information. Accurate diagnosis of lung sounds and their correlation with clinical findings can be a powerful tool in diagnosing lung diseases [8].

This study involves the use of lung sounds to diagnose and classify COPD through Machine Learning (ML) techniques with high accuracy. This method can be an effective tool to assist doctors and specialists in the field of health. ML is a suitable approach for disease prediction, decision-making, and diagnosis that does not require human intervention. This technique is rapidly growing in the medical industry, from disease diagnosis to medical imaging [9]. COPD is treated with lifestyle changes such as smoking cessation and breathing techniques, prescription medications such as bronchodilators and corticosteroids, supplemental oxygen therapy, and pulmonary therapy. For more severe cases, surgery is sometimes an option. Figure 1 shows a representation of the lung cycle for COPD patients.

This study aims to diagnose COPD and its severity by extracting appropriate features in the time-frequency domain resulting from the Stockwell transform (S-transform). The S-transform has a higher frequency resolution at low frequencies and a lower frequency resolution at high frequencies, but a higher time resolution. After extracting the feature using the S-transform, mathematical statistics have been applied to reduce the dimensions of the feature. The rest of the paper is organized as follows: Section 2 describes the literature review; Section 3 discusses the methods and materials; Section 4 collects the data; After that, Section 5 describes the results; Finally, Section 6 is the conclusion.

2. Related works

In recent years, several clinical studies have explored the potential use of artificial intelligence in medicine.

Examples include the assessment of changes in pulmonary function and their impact on the quality of life, the number of treatments performed on patients, the rate of hospitalization, mortality due to the disease, and patient satisfaction. In this context, special attention has been given to patients with COPD.

In 2020, Moll et al. [10] used a random forest algorithm with 30 clinical features as input to predict disease progression in patients with COPD. The most informative features were then used in a Cox regression analysis to predict mortality. It should be noted that this method was compared to other statistical and machine learning models. The models were trained on individuals with moderate-to-severe COPD from a subset of individuals in the COPD Genetic Epidemiology (COPDGene) study, and their predictive performance was evaluated on the remainder of individuals with moderate-to-severe COPD in COPDGene and the longitudinal COPD assessment to identify surrogate endpoints for predictive testing. The Machine Learning Mortality Prediction COPD (MLMP-COPD) model resulted in a C-index of ≥ 0.7 in COPDGene [10].

Levy et al. have presented their research on the possibility of automatic COPD diagnosis using continuous oximetry data analysis. Levy and colleagues hypothesize that patients exhibit specific COPD patterns or dynamics in their oximetry sets that, using the given information, may indicate these conditions. In this study, 350 patients were studied, trained with the help of a random forest classifier using the extracted features, and evaluated using nested cross-validation. A total of 8 COPD subjects out of 70 were misclassified. No severe cases were detected [11].

Spathis and Vlamos investigated clinical decision support systems in diagnosing and treating COPD. The results of the machine learning model in this study showed that, in the case of COPD, the Random Forest classifier outperforms other techniques with an accuracy of 97.7%. At the same time, the most prominent features for diagnosis include smoking, forced expiratory volume, age, and vitals. Classification is mandatory [12].

Kandaswamy et al. have described in an article that since the sound signals of the lungs are not constant, the conventional frequency analysis method is not very successful in diagnostic classification. This article deals with a new method of analyzing lung sound signals using wavelet transform and classification using Artificial Neural

Network (ANN). Lung sound signals were analyzed into frequency sub-bands using wavelet transform, and a set of statistical features was extracted from the sub-bands to show the distribution of wavelet coefficients. An ANN-based system, trained using a flexible backpropagation algorithm, was implemented to classify lung sounds into one of six categories: Normal, wheeze, crackle, squawk, stridor, or rhonchus [13].

In the study by Wi et al., a retrospective cohort study was used, which included 595. The plan was checked manually on a group to diagnose Asthma based on PAC. Then, in the next step, half of the data, i.e., 298 data points, were used as training data, and the rest of the samples were used as test data using the NLP-PAC algorithm. The data distribution was 160 men and 268 white women, and the average age was 2.3 years. Description, specificity, positive predictive value, and negative predictive value for the NP algorithm in predicting Asthma status were 92%, 96%, 89%, and 97%, respectively [14].

Using machine-based algorithms by Lu et al., such as regression, simple decision-making, and the perceptron algorithm, were used to predict the onset of severe Asthma in 2010 patients. However, the model based on logistic regression achieved 90% sensitivity and 83% specificity [15].

Prosperi et al. compared linear and non-linear models for predicting Eczema and Asthma. The method proposed in this study also follows this path and replaces Eczema with chronic lung disease COPD. They suggested that more complex modeling is the appropriate solution to better understand the mechanisms of illness and personal health care. They argued that in addition to performance, the system must be interpreted in terms of complexity. The experiments considered the mentioned opinions and provided the ability to interpret them by ranking the features. In this study, several factors were found to overlap in the diagnosis of Asthma and COPD. There was a higher level of sensitivity and specificity for non-linear models compared to other methods, particularly for Asthma and wheezing, with an area under the receiver operating characteristic curve of 84%, 76%, and 64%, respectively [16].

In Liu et al.'s paper, automatic seizure detection is essential for diagnosing epilepsy and reducing the extensive workload of reviewing continuous EEGs. This work proposes a new approach, combining S-transform with deep Convolutional Neural Networks (CNN), to detect the onset of seizures in long-term intracranial EEG recordings. The sensitivity obtained is 97.01%, and the accuracy is 98.12% [17].

In the article by Melekoğlu et al., for faster diagnosis of COPD and easier prevention of the disease, the use of the photoplethysmography (PPG) signal was applicable. This study aims to determine whether COPD can be diagnosed with PPG. Two groups of healthy and sick signals were investigated. Each group of signals was first cleaned with a numerical filter method of 0.1-20 Hz. Then, 25 feature extraction cases were performed in the time domain. According to the results, the highest performance values were obtained with 2 seconds data group and 99% sensitivity, 99% specificity, and 98.99% accuracy [18].

Palaniappan et al. [19] have described an article related to the analysis of lung sounds. At the beginning of the

features, identifying the distinctive features of a decision plays a major role in the classification of lung sounds. The features can be extracted from the signals in the time, frequency, and time-frequency domains. The feature techniques commonly used in computer-based lung sound analysis are the regression model, Mel frequency coefficients, energy, entropy, generative features, and wavelet. The use of wavelet-based features in Hurley et al.'s work has been the basis for 100% classification accuracy for the training set using ANN [20].

Khan et al. objectively analyzed lung sound signals associated with COPD. Specifically, Empirical Mode Decomposition (EMD), a data-adaptive signal decomposition technique suitable for analyzing non-stationary signals, was employed to decompose non-stationary lung acoustic signals. Applying EMD to the lung sound signal results in Intrinsic Mode Functions (IMFs) that are symmetric and band-limited. Analytical IMFs were then calculated through the Hilbert transform, which represents the instantaneous frequency content of each IMF. The Hilbert transform signal is analytic and has a complex representation including real and imaginary parts. Then, the Central Tendency Measure (CTM) was introduced to quantify the circular shape of the IMF analysis chart. The result was considered a useful feature for the diagnosis of normal lung sound signals with Amyotrophic Lateral Sclerosis (ALS). The simulation results show that the analytical CTM IMFs have a strong ability to discriminate between normal and ALS lung sound signals [21].

In this study, we aimed to diagnose and evaluate the severity of COPD based on the characteristics of the time and frequency of the S-transform applied to the pulmonary sound signal, which has not been widely studied for COPD diagnosis.

3. Material and methods

The general block diagram of the research is presented in Figure 2. According to this block diagram, first, the necessary filters are applied to the lung sound signal; then the primary features are extracted using the proposed of combine the Discrete Cosine Transform and Discrete Orthogonal Stockwell Transform (DCT-DOST) algorithm, and finally, the features are reduced through mathematical statistics. Then, class label classification is applied to K-Nearest Neighbors (KNN) and Support Vector Machine (SVM) classifiers.

4. Database

In this study, two stethoscopes were used to collect data through a clinical method. A Computerized Medical Instrumentation (CMI) database has been created with lung and heart sounds from patients with different stages of COPD, respiratory disorders such as Asthma and chronic bronchitis, and healthy breathing recordings from various individuals. Voluntary consent was obtained through a voluntary form with minimal information. Patients aged 38 to 68 years were selected from different occupational groups, socio-economic statuses, and male and female genders for the analysis of disorders. The studied population consists of 13 females and 64 males. The distribution of diseases according to gender is shown in Table 1.

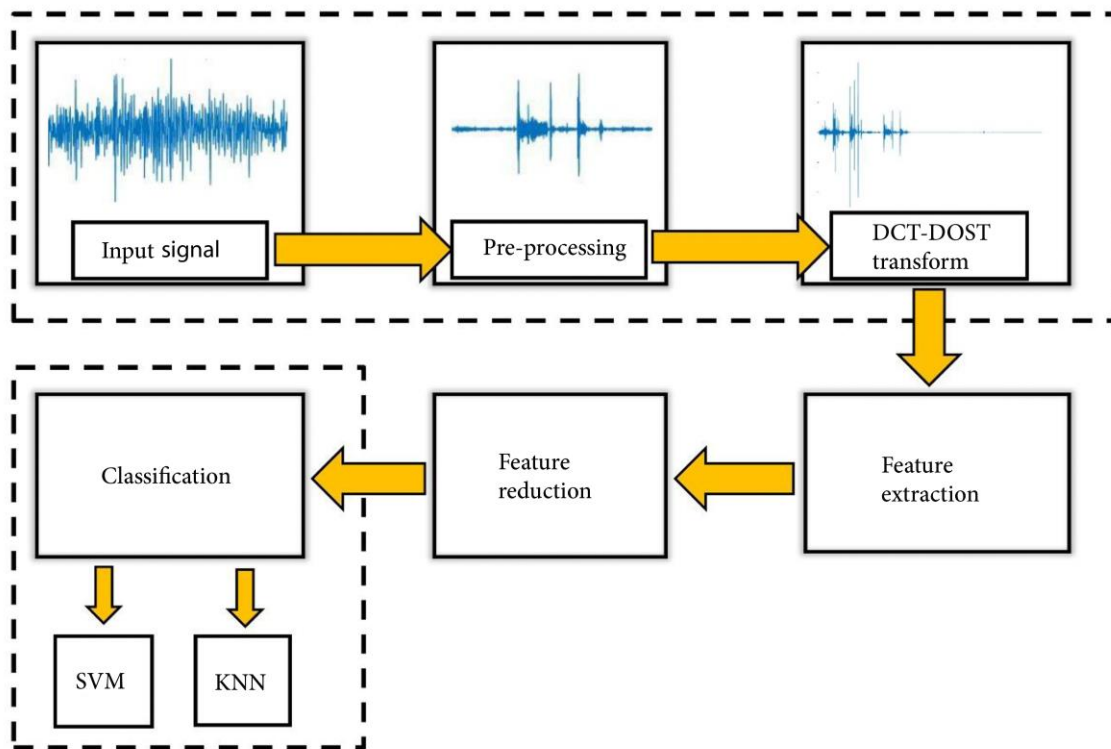


Figure 2. Block diagram of the proposed method.

Table 1. Diseases according to gender and their clinically diagnosed health status [22].

Diseases	Records	Gender	
		Male	Female
Asthma	6	4	2
COPD 0	5	4	1
COPD 1	5	4	1
COPD 2	7	7	-
COPD 3	7	6	1
COPD 4	17	13	4
Healthy	30	26	4
Total	77	64	13

During the study, healthy subjects and those with Asthma were excluded from the testing group, and only individuals with COPD were examined. As a result, the publicly available database only contained information on subjects with COPD, while the database for Asthmatic and healthy cases was excluded.

The 16-channel database was acquired with lung and heart auscultatory sounds collected from 8 basic foci on both sides of every subject. Simultaneous recordings from 2 channels for the left and right body regions were made for the TR@ respiratory database. However, parallel recording of 2-channel hearing aid sounds can cause deviations in milliseconds. The coordinator needs a distinct point to separate the start of two adjacent recordings. In this study, the patient was asked to cough for the first 5 seconds before starting to breathe to provide a clear separation between recordings. Coughing during auscultation can cause an unexpected increase in the sound signal. Peaks in specific areas of sound can be automatically detected using the built-in CMI and marked with an annotation bar.

Khan et al. also discusses the advantages of electronic stethoscopes over traditional stethoscopes, such as the

ability to record and analyze sounds, and the potential for telemedicine applications [22].

Despite the specifications of the digital stethoscope, which reduce 85% of ambient noise, artificial sounds such as room acoustics, contact noise from the doctor, and high-frequency movement can cause friction between the skin and the diaphragm, leading to unwanted noise. To remove any offset, lung sounds were filtered using a high-pass filter at 7.5 Hz (Butterworth first-order DC filter). In addition, a low-pass filter at 10 kHz (Butterworth 8th-order filter) was used to reduce aliasing and high-frequency noise during the analysis [23].

4.1. Pre-processing

In general, filtering is a necessary step before processing to remove noise and signal interference. In this database, filtering was done to remove unwanted noise and friction between the stethoscope's diaphragm and the skin. In this section, a secondary filter will be used to remove signal interference. The filter used in this research is a Butterworth filter.

In this database, the heart and lung signals can interfere with each other due to overlapping frequency ranges. The optimal frequency range of the lung signal is approximately 150 Hz to 2000 Hz, while the main frequency range of the heart signal is below 150 Hz [19]. To separate the two signals, a 4th-order Butterworth band-pass filter was used with a lower cut-off frequency of 150 Hz and an upper cut-off frequency of 1950 Hz.

The reason for using a 4th-order Butterworth filter is that increasing the order of the filter not only increases its sharpness but also causes a greater delay when applied. This results in increased computational requirements. Therefore, lower orders of the Butterworth filter are preferred, provided that the filter's cut-off frequency is

appropriate. In this study, a suitable cut-off frequency has been obtained using a 4th-order filter, and therefore there is no need to increase the order of the filter.

Due to the small number of subjects studied, each signal was divided into 3 segments to artificially increase the dataset, while maintaining the same label. This increased the number of samples from 59328 to 19776 per segment, and the number of samples increased from 42 to 126.

4.2. S-transform

The lung signal is a dynamic and non-static signal. As a result, a time-frequency transform is suitable for them. The transform studied in this research is the modified S-transform. In the following, the S-transform and its modifications will be introduced.

The S-transform retains the good properties of both the Short-Time Fourier Transform (STFT) and wavelet transform. The S-transform can be considered a wavelet transform that is phase-corrected, and from another point of view, it can be seen as a special mode of the STFT that uses a Gaussian window with a variable length. The length of this Gaussian function depends on the variance of the function, becoming wider as the variance increases and narrower as the variance decreases.

The S-transform is defined by determining the local spectrum at a specific time point ($t=\tau$) in a time series ($x(t)$). This is achieved by multiplying $x(t)$ with a Gaussian window, centered at $t=\tau$, and then taking the Fourier transform of the resulting product.

$$S(t, f, \sigma) = \int_{-\infty}^{+\infty} x(\tau)g(t-\tau, \sigma)e^{-j2\pi f\tau} d\tau. \quad (1)$$

In the original S-transform, a scaled Gaussian window called $g(t-\tau, \sigma)$ is used, with its midpoint at $\tau=t$. For any given time point t and frequency f , the S-transform can be considered a collection of localized Fourier coefficients. These coefficients are obtained by analyzing only the part of the primary function that lies within a few cycles on either side of $\tau=t$. As the frequency f increases, the relevant range of τ becomes more localized around t due to the scaled narrowing of the Gaussian window $g(t-\tau, \sigma)$.

For this purpose, variance is considered as a function of frequency. The variable length of the window makes the resolution variable with the frequency. The scaled Gaussian window $g(t-\tau, \sigma)$ where the middle point of this window is located at the point $\tau=t$, is in the form of Eq. (2):

$$g(t-\tau, \sigma) = \frac{1}{\sigma\sqrt{2\pi}} e^{\left(-\frac{(t-\tau)^2}{2\sigma^2}\right)}. \quad (2)$$

By choosing the variance as $\sigma = \frac{1}{|f|}$, the Gaussian window is calculated as Eq. (3). In Eq. (4), the Fourier transform of this Gaussian window is presented in terms of the variable τ .

$$g\left(t-\tau, \frac{1}{|f|}\right) = \frac{|f|}{\sqrt{2\pi}} e^{\left(-\frac{(t-\tau)^2 f^2}{2}\right)}. \quad (3)$$

When the Fourier transform of it is taken with respect to τ , which is also a Gaussian function, the resulting function is obtained:

$$G(v, f) = e^{\left(-\frac{2\pi^2 v^2}{f^2}\right)}. \quad (4)$$

Finally, S-transform of $h(t)$ signal can be expressed as Eq. (5):

$$ST(\tau, f) = \int_{-\infty}^{+\infty} h(t) \frac{|f|}{\sqrt{2\pi}} e^{\left(-\frac{(t-\tau)^2 f^2}{2}\right)} e^{-j2\pi ft} dt. \quad (5)$$

As the frequency increases, the length of the Gaussian window decreases and leads to an increase in the length of the window in the frequency domain. Thus, in the S-transform, the frequency resolution is better at low frequencies, and the frequency resolution is lower at high frequencies, but the time resolution is increased. This transform has weaker performance in detecting high frequencies than lower frequencies. To solve this issue, amendments have been proposed, which can be mentioned as changes [24, 25].

4.3. Discrete Orthonormal Stockwell Transform (DOST)

They provide an efficient method for computing the discrete canonical S-transform, DOST. DOST is a modified version of the S-transform that solves many memory and computing issues because Sin and Cos functions have been used [26]. In DOST, the input signal is displayed periodically. And while reducing the coefficients, it loses its shape.

For how to combine the transforms to obtain the DOST transform, we follow the path of Wang and Orchard. The following basis vector defined by Stockwell is a sum of the Fourier basis vector that is time-shifted and phase-corrected.

$$D_{v\beta\tau}[k] = \frac{e^{i\pi\tau}}{\sqrt{\beta}} \sum_{f=v-\beta/2}^{v+\beta/2-1} \exp\left(-i\frac{2\pi}{N}kf\right) \exp\left(+i\frac{2\pi}{\beta}\tau f\right). \quad (6)$$

In this context, f represents the frequency, while t and τ are both variables that correspond to time or space, and v is the center of the sub-block in the overall matrix. DOST is an orthogonal transform, and each coefficient is obtained by the inner product of the signal vector with a basis vector. Lastly, observe that the ultimate summation is an inverse Fourier transform applied to a sub-band of the Fourier change of the signal. Finally, β_k , τ_k , Ω_k are the bandwidth, time index, and bandwidth of the basis vector, respectively.

$$\begin{aligned} \langle h, D_{v\beta\tau} \rangle &= \sum_{k=0}^{N-1} h[k] \frac{e^{i\pi\tau}}{\sqrt{\beta}} \sum_{f=v-\beta/2}^{v+\beta/2-1} \exp\left(-i\frac{2\pi}{N}kf\right) \exp\left(+i\frac{2\pi}{\beta}\tau f\right) = \\ &= \frac{e^{i\pi\tau}}{\sqrt{\beta}} \sum_{f=v-\beta/2}^{v+\beta/2-1} \exp\left(+i\frac{2\pi}{\beta}\tau f\right) \sum_{k=0}^{N-1} h[k] \exp\left(-i\frac{2\pi}{N}kf\right) \\ &= \frac{e^{i\pi\tau}}{\sqrt{\beta}} \sum_{f=v-\beta/2}^{v+\beta/2-1} F(h) |f| \exp\left(+i\frac{2\pi}{\beta}\tau f\right), \end{aligned} \quad (7)$$

$$S[k] = \sqrt{\beta_k} e^{i\pi\tau k} \left(F_{\Omega_k}^{-1} F h\right)[k]. \quad (8)$$

The DOST is a variation of the general Fourier-family transform, but instead of a truncated Gaussian window, it

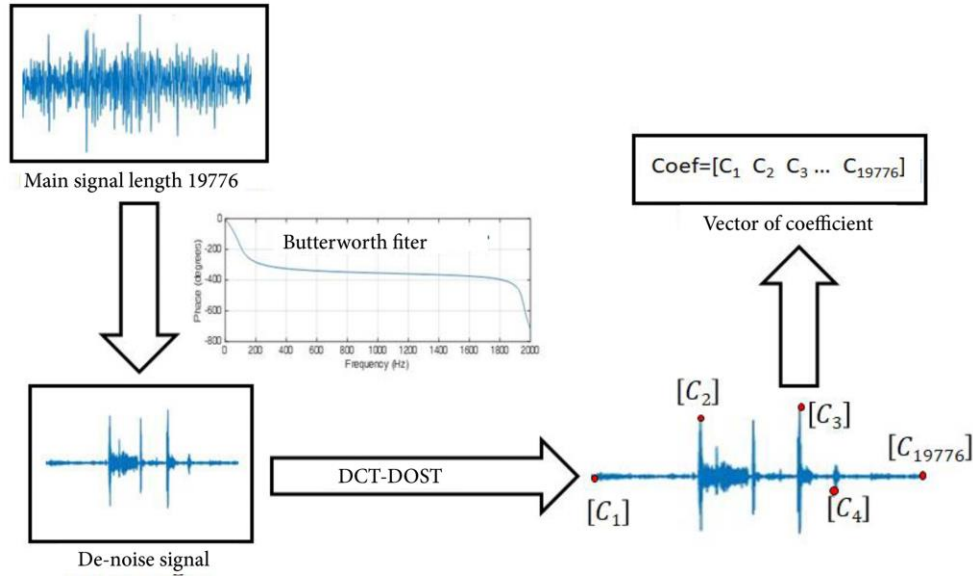


Figure 3. Block diagram of the DCT-DOST transform.

uses a rectangular window. In Eq. (10), a fast algorithm for the DOST is introduced, which can be modified to produce the conjugate-symmetric DOST as noted in Eq. (10). Another way to analyze the DOST is to view it in the context of matrices. It can be expressed as a matrix product. Finally, DOST can be considered in the framework of matrices:

$$DOST = \left(\oplus_{i=1}^K D_i \right) DFT, \quad (9)$$

$$D_i = \begin{bmatrix} 1 & 0 & \cdots & 0 \\ 0 & -1 & \cdots & 0 \\ \vdots & \vdots & \ddots & \vdots \\ 0 & 0 & \cdots & (-1)^n \end{bmatrix} F^{-1}. \quad (10)$$

The DOST transform is separable, so higher-dimensional transforms can be performed by applying the transform on each axis one after the other.

The discrete cosine transform is a real-valued transform, which makes it more suitable for compression and filtering. The connection of DCT-DOST with the Fourier transform makes it compatible with the DOST algorithm. A DCT-based DOST DCT-DOST may be defined simply by replacing the DFT in Eq. (9) with DCT:

$$DCT-DOST = \left(\oplus_{i=1}^K DCT_{ni}^{-1} \right) DCT. \quad (11)$$

Due to the advantages that the DCT transform has when compressing the initial coefficients and also because its coefficients are real, these two transforms have been combined, and DCT-DOST is presented. In the DCT transform, it can maintain the shape of the input signal while reducing the coefficients [27].

$$DCT-DOST = \left(\oplus_{i=1}^k DCT_{\eta_i}^{-1} \right) DCT. \quad (12)$$

Finally, due to the higher calculation speed and the accuracy of the coefficients, S-transform corrections (DCT-DOST) have been used.

4.4. Feature extraction

After applying the necessary filters and obtaining the raw signal, the desired transform is applied to the signal. In this

research, the DCT-DOST transform was used, which was applied to the lung sound signals, and the resulting coefficients were obtained as shown in Figure 3.

In the DCT-DOST transform, the number of coefficients is equal to the number of signal samples and its value is 19776. The number of features is 19776. To reduce the dimensionality of the feature space, mathematical parameters such as mean, mode, max, min, kurtosis, skewness, Standard Deviation (STD), variance, range, Root Mean Square (RMS), median, and mode were used. This reduced the number of features to 14, as shown in Figure 4, which illustrates the general process of feature selection.

5. Results

The validation method used in this study is K -fold, and we will discuss its properties below. The following results of validation using KNN and SVM methods are observed and evaluated.

Classification means labeling areas based on similar characteristics of signals. The purpose of this research is to implement the KNN and SVM algorithms in order to compare the accuracy of feature classification. In this article, due to the strong features extracted from DCT-DOST, a classifier with high speed and a smaller number of mathematical calculations is used, which is the main point of the article. KNN calculates the distance between a test data point and each training data point using a distance metric such as Euclidean or Manhattan distance. It then selects the K closest neighbors and assigns the test data point to the majority class or the mean of their respective labels. The choice of distance metric can have a significant impact on the performance of the algorithm.

SVM stands for SVM, a powerful ML algorithm used for classification or regression tasks. SVMs use a kernel function to transform the input data into a high-dimensional feature space, where a linear decision boundary can be used to separate the classes. The choice of kernel function can have a significant impact on the performance of the algorithm.

In KNN classification, Hamming distance had better results compared to SVM, Hamming, Euclidean, Chebyshev,

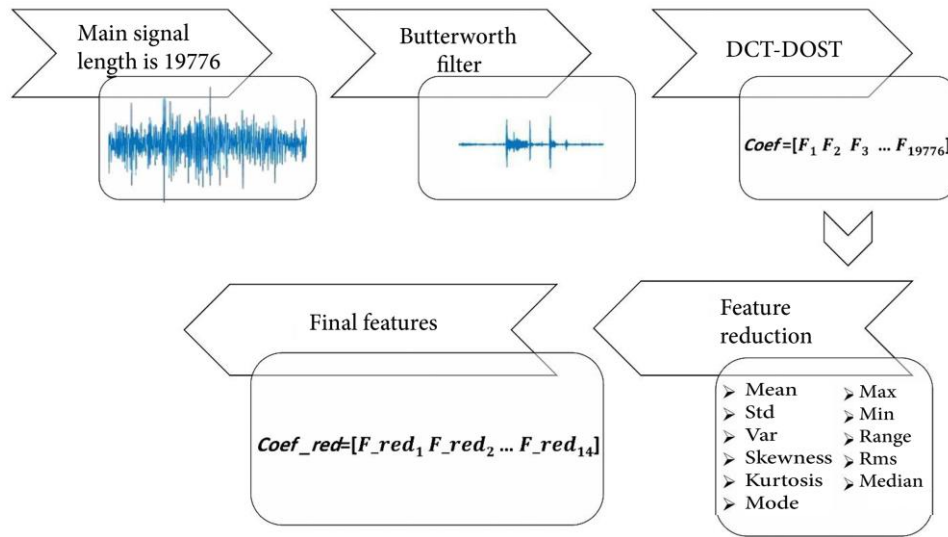


Figure 4. Schematic of feature reduction.

correlation, and Minkowski distances, and the number of neighborhoods from 1 to 10 was used with trial and error. As the results show, the percentage of results decreased with the increase in the number of neighborhoods.

In the K -fold method, there is a single parameter called K , which refers to the number of groups into which a given data sample is to be divided. As a result, this method is often referred to as K -fold validation. The goal of K -fold validation is to achieve a model with optimal parameter values. Model parameters are estimated using training data, while model error estimation is calculated based on validation data. After designing and building a model or algorithm, one of the most important steps is to evaluate its performance, accuracy, and correctness. In this study, the criteria of sensitivity, specificity, precision, and accuracy have been used to evaluate the classification and distinguish the classes, which are briefly shown in Box I.

In the KNN classifier, the best number of neighbors and distance, as well as in the SVM classifier, the best kernel and number of neighbors were obtained experimentally using K -fold evaluation methods.

As shown in Figure 5, the percentages obtained from the KNN classification with 5 different distances and the number of neighbors is from 1 to 5. As Figure 5 shows, the results decrease with the increase in the number of neighbors.

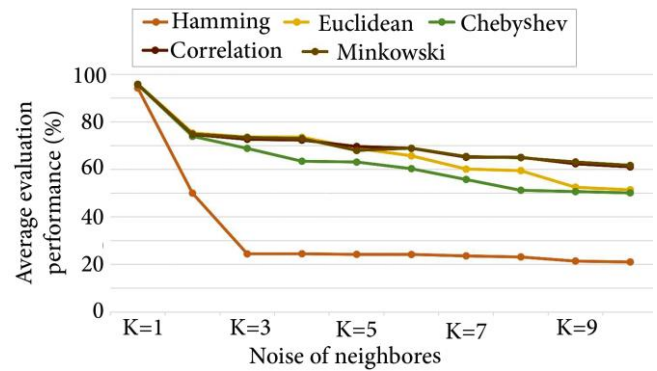


Figure 5. The average result (sensitivity, specificity, precision and accuracy) of five different distances for neighborhood numbers 1 to 10 with the KNN classifier.

$$\text{Accuracy} = \frac{\text{True positive} + \text{True negative}}{\text{True positive} + \text{False negative} + \text{False positive} + \text{True negative}}, \quad (13)$$

$$\text{Sensitivity} = \frac{\text{True positive}}{\text{True positive} + \text{False negative}}, \quad (14)$$

$$\text{Specificity} = \frac{\text{True negative}}{\text{True negative} + \text{False positive}}, \quad (15)$$

$$\text{Precision} = \frac{\text{True positive}}{\text{True positive} + \text{False positive}}. \quad (16)$$

- True Positive (TP): A test result that correctly indicates the presence of a condition or specificity;
- True Negative (TN): A test result that correctly indicates the absence of a condition or specificity;
- False Positive (FP): A test result that wrongly indicates that a particular condition or attribute is present;
- False Negative (FN): A test result that wrongly indicates that a particular condition or attribute is absent.

		Predict		TOTAL	
Actual		True positive	False neative		
		95	1	96	Accuracy= 96.03% Std = ± 2.42
	False positive	4	True negative	30	Precision=96.30% Std = ± 3.09
			26		
TOTAL		99	27	126	
		Sensitivity= 95.96% Std = ± 2.08			

Figure 6. Total confusion matrix for five classes by applying the S transform in the KNN classifier.

Table 2. The results of the SVM classifier.

Kernel	SEN (%)	SPE (%)	ACC (%)	PRE (%)
Polynomial	83.33	95.23	92.59	83.33
Linear	67.46	89.23	83.82	67.46
RBF	76.98	93.04	89.31	76.98

As a result, for all distances, the number of neighbors 1 shows the best result.

The results shown in Figure 5, with the data used in this study with the KNN classification, decrease from neighborhood Number 1 to neighborhood Number 5; in all distances, the best result is for the Euclidean distance with neighborhood Number 1.

Figure 6 shows the confusion matrix of the KNN classifier. Due to 10 repetitions, the confusion matrix exhibits slight changes, which are represented by the STD.

Table 2 displays the results of SVM classification performed using three different kernels: Linear, polynomial, and Radial Basis Function (RBF).

Table 2 indicates that the polynomial kernel achieved the highest performance, while the linear kernel obtained the lowest performance.

Figure 7 illustrates that the KNN classifier with Euclidean distance and neighborhood 1 achieved better results than the SVM classifier with the polynomial kernel. This research aims to diagnose and evaluate COPD from the lung signal with 5 different severities from COPD0 to COPD4 using the time-frequency transform of the S-transform. Several tests and methods have been performed to improve the general and partial results to achieve the best classification accuracy. At first, after equalizing the length of the lung signal and performing the required pre-processing, including filtering the interference in the signal, the S-transform was applied to the data to extract features.

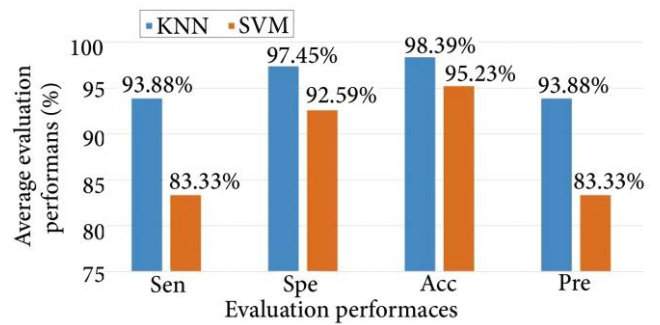


Figure 7. The average result (sensitivity, specificity, precision, and accuracy) of KNN and SVM classifiers.

Due to a large number of signal samples and the same number of coefficients obtained from the samples, feature dimension reduction has been used using mathematical statistics, reducing the number of coefficients from 19776 to 14 features. Now, to diagnose and evaluate the different severities of this disease, the features have been applied to KNN and SVM classification, which was done in KNN using the K-fold validation method.

The main goal of this study is to use the S-transform to extract features from lung sound signals for COPD diagnosis. Using the KNN classifier with different distances and the number of neighbors from 1 to 10, and the SVM classifier with different kernels, the best results were obtained by trial and error, which shows the superiority of the KNN classifier compared to SVM. By using the KNN classifier, good results were obtained in the accuracy, sensitivity, and precision evaluation criteria.

According to the investigations carried out in the KNN classifier with K-fold validation with $k=10$ and the number of neighbors 1 and the Euclidean distance, with 97.45% accuracy, 98.39% accuracy, and 93.88% sensitivity, the best results among others have evaluation methods were obtained. Table 3 shows the proposed algorithm performed in this study with other methods.

6. Conclusion

In this study, real coefficients and primary features were extracted using the time-frequency Stockwell transform (S-transform) and its modification based on the Discrete Cosine Transform and Discrete Orthogonal Stockwell Transform (DCT-DOST). By applying the statistical features to the primary features, a very significant reduction in the dimensions of the features to 14 features was achieved. The results of the 5-class classification show the effective feature space in the classification of Chronic Obstructive Pulmonary Disease (COPD) disease severity.

Table 3. Comparison of previous works using the lung sounds database with the proposed method.

Authors	Signal type	Channel	Method	Classifier	SPE (%)	SEN (%)	ACC (%)
Sánchez Morillo et al. [28]	Tracheal sound	1	STFT	NN	81.80	72.00	77.60
Altan et al. [29]	Lung sound	12	3D-SODP	DBN	93.65	93.34	95.84
Kim et al. [30]	Lung sound	-	VGG16	SVM	85.70	82.30	82.40
Purpose method	Lung sound	12	DCT-DOCT	KNN	98.39	93.88	97.45

Compliance with ethical standards

Research Involving Human Participants and/or Animals

This paper does not contain any studies with human participants or animals performed by any of the authors.

Informed Consent

Informed consent was obtained from all individual participants included in the study.

Funding

This research did not receive any specific grant from funding agencies in the public, commercial, or non-for-profit sectors.

Conflicts of interest

The authors declare that they have no known competing financial interests or personal relationships that could have appeared to influence the work reported in this paper.

Authors contribution statement

First author: Writing the article; Editing the text; Programming; and performing the required analyses for the research.

Second author: Supervisor of this research; Ideation and initial design of the study and provided effective participation and guidance in the editing; Scientific review; and final improvement process of the article.

References

- Lareau, S.C., Fahy, B., Meek, P., et al. "Chronic Obstructive Pulmonary Disease (COPD)", *Am. J. Respir Crit. Care. Med.*, **199**(1) (2019). <https://doi.org/10.1164/rccm.1991p1>
- Vogelmeier, C.F., Román-Rodríguez, M., Singh, D., et al. "Goals of COPD treatment: Focus on symptoms and exacerbations", *Respir Med.*, **166**, 105938 (2020). <https://doi.org/10.1016/j.rmed.2020.105938>
- Ritchie, A.I. and Wedzicha, J.A. "Definition, causes, pathogenesis, and consequences of chronic obstructive pulmonary disease exacerbation", *Clin. Chest. Med.*, **41**(3), pp. 421-438 (2020). <https://doi.org/10.1016/j.ccm.2020.06.007>
- Li, J, Sun, S., Tang, R., et al. "Major air pollutants and risk of COPD exacerbations: A systematic review and meta-analysis", *International Journal of Chronic Obstructive Pulmonary Disease*, **11**(1), pp. 3079-3091 (2016). <https://doi.org/10.2147/copd.s122282>
- Iheanacho, I., Zhang, S., King, D., et al. "Economic burden of Chronic Obstructive Pulmonary Disease (COPD): A systematic literature review", *Int. J. Chron Obstruct Pulmon Dis.*, **15**, pp. 439-460 (2020). <https://doi.org/10.2147/copd.s234942>
- Stocks, J. and Sonnappa, S. "Early life influences on the development of chronic obstructive pulmonary disease", *Therapeutic Advances in Respiratory Disease*, **7**(3), pp. 161-173 (2013). <https://doi.org/10.1177/1753465813479428>
- Padilla-Ortiz, A.L. and Ibarra, D. "Lung and heart sounds analysis: State-of-the-art and future trends", *Crit. Rev. Biomed Eng.*, **46**(1), pp. 33-52 (2018). <https://doi.org/10.1615/critrevbiomedeng.2018025112>
- Loudon, R. and Murphy, R.L. "Lung sounds", *Am. Rev. Respir Dis.*, **130**, pp. 663-73 (1984).
- Battineni, G., Chintalapudi, N., and Amenta, F. "Machine learning in medicine: Performance calculation of dementia prediction by support vector machines", *Informatics in Medicine Unlocked*, **16**, 100200 (2019). <https://doi.org/10.1016/j.imu.2019.100200>
- Moll, M., Qiao, D., Regan, E.A., et al. "Machine learning and prediction of all-cause mortality in COPD", *Chest*, **158**(3), pp. 952-964 (2020). <https://doi.org/10.1016/j.chest.2020.02.079>
- Levy, J., Álvarez, D., del Campo, F., et al. "Machine learning for nocturnal diagnosis of chronic obstructive pulmonary disease using digital Oximetry biomarkers", *Physiol. Meas.*, **42**(5), 054001 (2021). <https://doi.org/10.1088/1361-6579/abf5ad>
- Spathis, D. and Vlamos, P. "Diagnosing Asthma and chronic obstructive pulmonary disease with machine learning", *Health Informatics Journal*, **25**(3), 1460458217723169 (2019). <https://doi.org/10.1177/1460458217723169>
- Kandaswamy, A., Kumar, C.S., Ramanathan, R.P., et al. "Neural classification of lung sounds using wavelet coefficients", *Computers in Biology and Medicine*, **34**(6), pp. 523-537 (2004). [https://doi.org/10.1016/S0010-4825\(03\)00092-1](https://doi.org/10.1016/S0010-4825(03)00092-1)
- Wi, C.-I., Sohn, S., Ali, M., et al. "Natural language processing for Asthma ascertainment in different practice settings", *The Journal of Allergy and Clinical Immunology: In Practice*, **6**(1), pp. 126-131 (2018). <https://doi.org/10.1016/j.jaip.2017.04.041>
- Lu, M.T., Ivanov, A., Mayrhofer, T., et al. "Deep learning to assess long-term mortality from chest radiographs", *JAMA Network Open*, **2**(7), 197416 (2019). <https://doi.org/10.1001/jamanetworkopen.2019.7416>
- Prosperi, M.C., Marinho, S., Simpson, A., et al. "Predicting phenotypes of Asthma and Eczema with machine learning", *BMC Medical Genomics*, **7**, pp. 1-10 (2014). <https://doi.org/10.1186/1755-8794-7-s1-s7>
- Liu, G., Zhou, W., and Geng, M. "Automatic seizure detection based on S-transform and deep convolutional neural network", *International Journal of Neural Systems*, **30**(4), 1950024 (2020). <https://doi.org/10.1142/S0129065719500242>

18. Melekoğlu, E., Kocabiçak, Ü., Uçar, M.K., et al. "Machine learning for the diagnosis of chronic obstructive pulmonary disease and photoplethysmography signal-based minimum diagnosis time detection", In *Trends in Data Engineering Methods for Intelligent Systems*, **76**, pp. 42-58 (2021). https://doi.org/10.1007/978-3-030-79357-9_6
19. Palaniappan, R., Sundaraj, K. and Ahamed, N.U. "Machine learning in lung sound analysis: A systematic review", *Biocybernetics and Biomedical Engineering*, **33**(3), pp. 129-135 (2013). <https://doi.org/10.1016/j.bbe.2013.07.001>
20. Hurley, N.C., Spatz, E.S., Krumholz, H.M., et al. "A survey of challenges and opportunities in sensing and analytics for cardiovascular disorders", *CM Trans. Comput Healthc.*, **2**(1), pp. 1-42 (2019). <https://doi.org/10.1145/3417958>
21. Khan, S.I., Kumar, G.G., Naishadkumar, P.V., et al. "Analysis of normal and adventitious lung sound signals using empirical mode decomposition and central tendency measure", *Treatment du Signal*, **38**(3), pp.731-738 (2021). <https://doi.org/10.18280/ts.380320>
22. Khan, S.I., and Ahmed, V. "Study of electronic stethoscope as prospective analysis tool for cardiac sounds", In *Smart Trends in Information Technology and Computer Communications: First International Conference*, **628**, pp. 706-713 (2016). https://doi.org/10.1007/978-981-10-3433-6_85
23. Altan, G., Kutlu, Y., Garbi, Y., et al. "Multimedia respiratory database (RespiratoryDatabase@ TR): Auscultation sounds and chest X-rays", *Natural and Engineering Sciences*, **2**(3), pp. 59-72 (2017). <https://doi.org/10.48550/arXiv.2101.10946>
24. Assous, S. and Boashash, B. "Evaluation of the modified S-transform for time-frequency synchrony analysis and source localization", *EURASIP Journal on Advances in Signal Processing*, **2012**, 49 (2012). <https://doi.org/10.1186/1687-6180-2012-49>
25. Khan, S.I. and Ahmed, V. "Study of effectiveness of Stockwell transform for detection of coronary artery disease from heart sounds", In *2nd International Conference on Contemporary Computing and Informatics (IC3I)*, pp. 725-728 (2016). <https://doi.org/10.1109/IC3I.2016.7918056>
26. Wang, Y. and Orchard, J. "Fast discrete orthonormal Stockwell transform", *SIAM Journal on Scientific Computing*, **31**(5) (2009). <https://doi.org/10.1137/080737113>
27. Raj, S. and Chandra Ray, K "ECG signal analysis using DCT-based DOST and PSO optimized SVM", *IEEE Transactions on Instrumentation and Measurement*, **66**(3), pp. 470-478 (2017). <https://doi.org/10.1109/TIM.2016.2642758>
28. Sánchez Morillo, D., Leon Jimenez, A., and Moreno, S.A. "Computer-aided diagnosis of pneumonia in patients with chronic obstructive pulmonary disease", *Journal of the American Medical Informatics Association*, **20**, pp. 111-117 (2013). <https://doi.org/10.1136/amiajnl-2012-001171>
29. Altan, G., Kutlu, Y., Pekmezci, A.Ö., et al. "Deep learning with 3D-second order difference plot on respiratory sounds", *Biomedical Signal Processing and Control*, **45**(1), pp. 58-69 (2018). <https://doi.org/10.1016/j.bspc.2018.05.014>
30. Kim, Y., Hyon, Y., Jung, S.S., et al. "Respiratory sound classification for crackles, wheezes, and rhonchi in the clinical field using deep learning", *Scientific Reports*, **11**, 17186 (2021). <https://doi.org/10.1038/s41598-021-96724-7>

Biographies

Saeid Rashidi was born in Tehran, Iran, in 1973. He received the PhD degree in Biomedical Engineering from the Amirkabir University of Technology, Tehran, Iran, in 2013. Currently, he is an Assistant Professor in the Faculty of Medical Sciences and Technologies, Science and Research Branch, Islamic Azad University. His research activities are concentrated in the areas of biomedical signal and image processing, biometrics, motor control, and chaos.

Mahsa Amin Eskandari was born in Tehran, Iran, in 1996. She received a bachelor's degree in Medical Engineering from the Islamic Azad University of Tehran, branch of medical sciences, in 2019. She is a graduate of Medical Engineering, majoring in Bioelectricity, from the Faculty of Medical Sciences and Technologies, Islamic Azad University, Science and Research branch. Her research activities are concentrated in the areas of biomedical signals, image processing, and machine learning.